

# Planning Method for Safety Neurosurgical and Computed Tomography Contrast-Data Set Visualization

**Avrunin OG<sup>1</sup> and Husham Farouk IS<sup>2\*</sup>**

<sup>1</sup>Kharkov National University of Radio Electronics, Lenina14, Ukraine

<sup>2</sup>INAYA Medical College, Saudi Arabia

**\*Corresponding author:** Husham Farouk Ismail Saied, 3. INAYA Medical College, Riyadh- Saudi Arabia, P.O. Box 271880, 11352, Saudi Arabia, Email: hushamfarouk@yahoo.com

**Research Article**

Volume 2 Issue 1

**Received Date:** January 09, 2019

**Published Date:** February 22, 2019

## Abstract

Discussed the issues' associated with the development of a computed neurosurgery planning system. An important part is to determine the value of invasive surgical access. The study purpose is to design a methodology for finding the shortest distance between surgical target and peripheral point of the brain tissue with strict adherence considering the type of the brain anatomical structure existing in the path of surgical track (risk map), these two condition used in companion to determine the risk value of the surgical access. The study method consists of two algorithms for calculating the shortest surgical access to the target and assuring the safety by avoiding high-density tissues identification method "internal map" describing the anatomy of the brain such as bones. An algorithm for automatic identification of brain vascular system also was designed. The structural diagram of the contrast data visualization system, using computed tomography data, was thoroughly discussed. Also, trying to contribute in solving issues facing developers of modern medical imaging visualization systems to select the most appropriate method from the whole arsenal of algorithms and processing models concerning displaying brain surgical zone using image registration and optical tracking system. The visualization of the target zone is carried out according to an internal reference landmark points inside the center of the brain as well as an automatic algorithm for contour recognition was applied. Moreover, the optical tracking system was used to assess the navigation accuracy of determining the position of the surgical instrument outside the patient head. Algorithms necessary for operational planning also was included, and the proposed method was applied in a pilot study with simulation mode to human brain model, in order to target a specific surgical zone, and as a result, the system suggested (24) possible surgical track, among them, were selected the best and safest access. The total error of a surgical instrument targeting was less than 3 mm (in average 2.6 mm).

**Keywords:** Data visualization; Data processing and displaying; Planning system; Specific surgical access; Risk map

## Introduction

The rapid development of medical technology, and in particular, eternal imaging graph equipment, modern neurosurgery leads to a qualitatively new level. Using current intelligent imaging techniques, in addition to identifying structural abnormalities (defects, injuries), and in some degree allow to determine the characteristics of anatomical of brain structure, and, as a consequence, take these parameters into account when choosing surgical access approaches.

Modern medical computer diagnostic system must provide clinical aid when carrying out a diagnosis to perform routine surgical operations and complex computational procedures, expanding the possibility of the investigation methods [1]. The improvement of data displaying methods in the field of medical imaging systems has a paramount importance that can significantly increase the efficiency of the diagnosis process [1,2]. The last 30 years were characterized by a rapid revolution in the improvement of radiation-mapping tools, such as X-ray, CT scan, magnetic resonance and positron emission tomography, and the main purpose of the diagnostic task anyway is to obtain the maxim information with a minimal patient injury [3,4].

Modern neurosurgical visualization systems clearly hold the principle of harmonization between hardware and software. It is important for the pre-planning of surgical intervention to select exactly methods (scanning modes control) that would be most informative and would allow obtaining the initial data with minimal instrumental errors. The software functions are assigned with the secondary data processing and resulting data visualization of the studied objects. The efficacy of the diagnosis method is associated with the possibilities of supporting algorithm and its software realization [5].

## The Relevance of the Study

Computed planning systems used for modern neurosurgery intervention are widely used in medical practice. This is primarily due to the complexity of calculating a reliable targeting approach that would lead to the most positive outcome of the intervention. At the same time, the planning system can solve these complex calculations by taking on itself a significant part of these tasks.

This study is trying to contribute to solving issues facing developers of modern medical imaging visualization systems to select the most appropriate

method from the whole arsenal of algorithms and processing models concerning displaying brain surgical zone. Also, the visualization of complex brain tissues was presented. An algorithm for automatic identification of brain vascular system was designed.

## Analysis of the Research and Literature

The use of commercial computer systems for neurosurgery planning widely covered in different literature [6-9]. Practical tasks are implemented abroad [9-12].

The neurosurgical planning, especially when performing interventions in deep-seated intracerebral structures, requires knowing not only the spatial arrangement of target regions, but also localization of vascular system and sinuses. While visualizing the vascular system, average data from specialized anatomical brain atlases are utilized, that, unfortunately, couldn't accurately investigate the vessels, owing to the high-individual variability of blood vessels [13,14]. The complex approach based on combining standard data from the angiographic and tomography examination usually leads to the reduction of accuracy of virtual visualization procedures, casing by the errors in reference orientation point's determination.

At the current stage, the most preferred method for modeling of the human brain vascular system is the spiral CT of contrast data visualization [15-17]. The essence of this method is based on a high-speed spiral brain scan, with an injection of special intravenous vital stain, permitting more contrast of the vascular channel through establishing a gradient concentration, between the intravascular and the extracellular spaces. The resulting CT-picture of the brain is extremely intricate to analyze and to investigate even by an experienced specialist. Therefore, in advance, it is urgent to solve the problem with means of carrying out the virtual visualization of a vascular channel with the possibility of interactive selection of the options for real-time monitoring and the required measuring procedures. The methods of data-mapping with computed tomography contrast data are divided into two approaches; 2D and 3D. The design and exploitation issues, the convenient software and the methods of tomography data processing were discussed in many pieces of literature [18-20]. However, the unresolved issues are related to the automatic segmentation procedure of the vascular channel, designing "smart" rendering algorithms and the optimization of surgical approaches based on data describing the location of vessels, taking into account the

anatomical variability. Hence, the actual modern tasks are aimed at developing computational methods and algorithms to achieve the maximum reality and visibility.

### Statement of the Problem and the Purpose of the Study

Development of a computer system planning neurosurgery is a major challenge. With its development raises an important issue related to the definition of the risk of interference particular surgical approach. This is largely mediated planning system determines the quality and consequently determines the outcome of the operation, the rate of a minimal patient injury, etc. The aim of this work is to study the various methods and approaches to identify invasive neurosurgical approaches (the access toward the target) and from them chose the best one.

The stereotactic calculation is considered as a high-precision guidance of a surgical instrument to the stereotactic target. For this purpose, the following must be considered:

- ❖ Create a 3D model of the human brain fulfill with the neurosurgical simulation.
- ❖ Image registration and tracing: by mean of matching of brain coordinate systems (target and reference landmarks) with a stereotactic apparatus.

- ❖ Formation of control parameters for the stereotactic apparatus (neurosurgical planning method).
- ❖ CT contrast data visualization as well as the implementation of special functional modules, carrying out CT data secondary processing, and intracerebral vessels visualization.

### Methods

#### The Structure of a Computed Neurosurgery Planning System

The methods were designed to perform surgical simulation and planning techniques for best surgical procedures (case study). In order to upgrade the capabilities of computed tomography (CT) systems, the generalized diagram of the computer planning system for a neurosurgical access was designed (Figure 1). CT study data will be loaded to the system in volumetric format data set, this data reformed according to a specific technique (this technique will be presented ahead), and these data used to build the 3D mathematical model and the common coordinate system. Based on this new model, the target zone will be identified and the surgical access track will be to construct according to two criteria. The neurosurgical planning, especially when performing interventions in deep-seated intracerebral structures, requires knowing not only the spatial arrangement of target regions but also localization of vascular system and neural tissue.

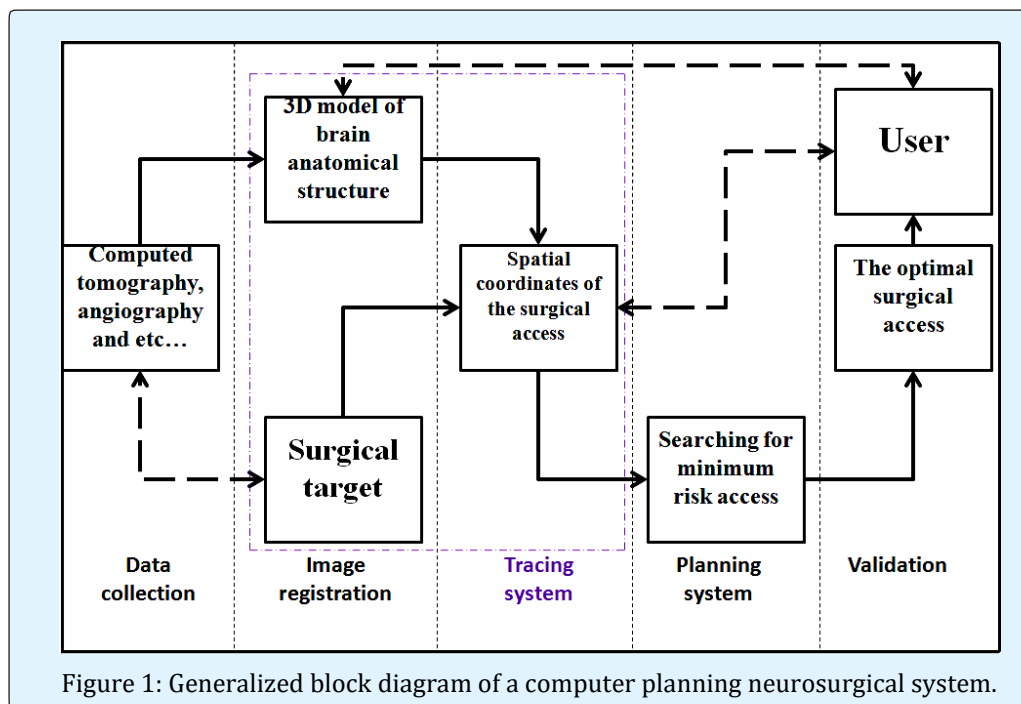


Figure 1: Generalized block diagram of a computer planning neurosurgical system.

The ultimate goal of designing of this system is to choose the best track(s) to reach the surgical target zone during a surgical intervention, targeting access will be calculated and selected from among number of tracks proposed by the system itself (possible tracks for surgical access) [20-22]. In general, the main elements of the frameless stereotaxy navigation systems in this study include the following:

### Image Registration and Tracking System

The position detection subsystems in the surgical navigation method should provide of two main functional procedures:


- Detection of surgical tool position (in/outside of patient head).
- Detection of patient head position.

The image registration based on image processing and transforming into a common coordinate system. The image registration is the main element of neuro-navigation procedures. To guide the frameless stereotactic navigation tool it's important to merge all data into a common model coordinate system, especially when multiple modalities and intraoperative imaging data are incorporated into the navigational plan.

In this study the detection of the surgical tool position inside of the patient head relies on technique based on spatial registration anatomic reference landmark, these

landmarks is carried out according to an algorithm for finding a points inside the center of the human brain, the automatic algorithm based on contour recognition, that is applied to edge the contour of the reference landmark point. The visualization is chosen to identify the (III ventricle) at the central intra-cerebral, to be as our reference point, which is necessary to localize the center of our stereotactic coordinate system. Details of this process are described in our previous work [23].

The summary of the proposed method is as follows: The target zone structure which will be a subject of destruction or simulation, is characterized by metastasis state and in the operative environment to be an identical landmark (III ventricle, Figures 2a & b) in a 3D model. The contrast of this structure (target zone), usually is unclear and cannot be visualized on the CT slice by using standard method. In this case, we used an indirect method of visualization for a surgical zone by linking in a common coordinate system, the localization of the (target zone) to the reference landmark point (III ventricle) inside the center of the brain. The reference point is described determined in the central point of the line connecting the anterior/posterior points of the third ventricle at the ventricular system. Detection of the reference point is based on CT scanning at the orbit metal line of the skull plane, this line passes through the posterior edge and external auditory meatus parallels to the middle line of (A-P) by an angle of deviation less than  $5^\circ$  [11,15].

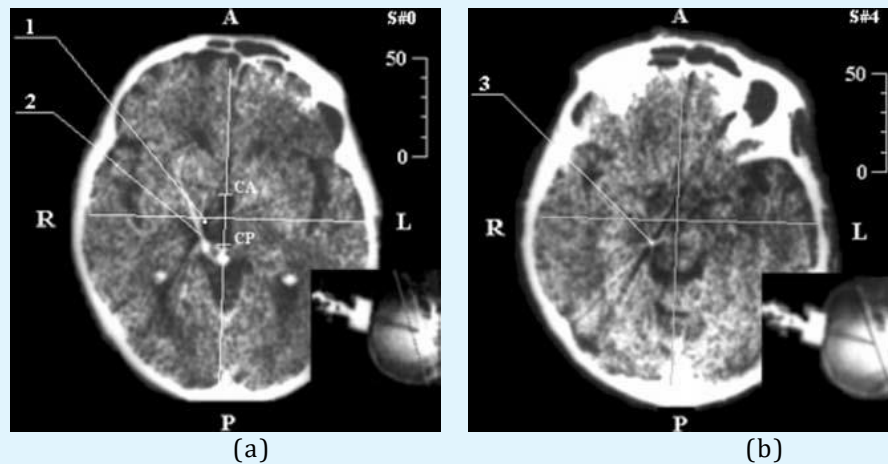

**Figure 2a:** Demonstration of neurosurgery CT-steretactic calculation, while targeting med-nucleus of colorless ball:

- a). stereotactic CT-slice at zero-plane level,
- b). CT- steretactic calculation at the level of surgical zone:
  1. The calculation of central point stereotactic-target zone,
  2. Artifact of cannula movement,
  3. Distal point of the cannula moving part.

**Figure 2b:** Anterior portion of third ventricle

Detection of surgical tool position outside of patient head is based on the spatial coordinates of anatomic external landmarks and optical position determination technology and estimation the sources of errors, this system was implementing and approved in our previous work [23]. The optical method of detecting surgical tool position can be summarized in the following: The tracking systems utilize on dual optical cameras that track the position of surgical tool relative to a fixed reference landmarks ( $m_1^1, m_1^1, m_{mn}^1, m_2^2, m_2^2, m_{mn}^2$ ). At first, consider the operation principle of the surgical instrument tracking and the patient's head position by using the optical approach. The method based on registration of the spatial location of the marker position by two optical cameras (Figure 3a), an example (Figure 3b).

A simplified functional block diagram of the operation principle of the surgical instrument position calculation using two-camera system was considered [23]. Two identical video detection devices are used for a surgical zone (v) detection and instrument position. Tracking: In order to extract complex instrument movement and patient's head position precisely, two cameras are used to capture the multi-view sequences. For each projection are made a calculations markers position ( $m_1^1, m_1^1, m_{mn}^1, m_2^2, m_2^2, m_{mn}^2$ ). The obtained data of matrix calculation are from the tool position transformation or patient head position as in refer to Tymkovich MY [24], these data describing the main stages of surgical instrument position in 3D coordinate system space. In the common positioning markers block, where made the common markers position determination in the space ( $M_{mn}, M_1, M_1$ ). According to the multi-view data projection+ the data coming from the matrix projection (C1, C2). Errors estimation and calibration: tracking of instrument movement can be achieved by virtue of the multi-view video sequences. The errors that occurred during tracking can be solved with the multi-view mode. Multiple views mean that the same video-view is captured with the same markers ( $m_1^1, m_1^1, m_{mn}^1, m_2^2, m_2^2, m_{mn}^2$ ) from different viewpoints, and the multiple corresponding image feature points are competent for reconstructing 3D coordinates of feature points accurately. Therefore, compared with monocular video sequence, 3D reconstruction is easier under multi-viewpoints. However, for each video-device were made a systematic calibration procedure, which were made to determine the surgical tool position using the projection matrix. The number of detected markers is equal to (mn), this number should be in full extent useful for determining the surgical

instrument position. Recognition: The information in the (model), describing the common positioning of markers ( $m_1^1, m_1^1, m_{mn}^1, m_2^2, m_2^2, m_{mn}^2$ ) in the object coordinate system, and transmit to final block, in order for determine the transformation matrix of the tool position (Ti), which refer to the position of surgical tool.



Figure 3a: Dual optical cameras used for surgical tool position determination.

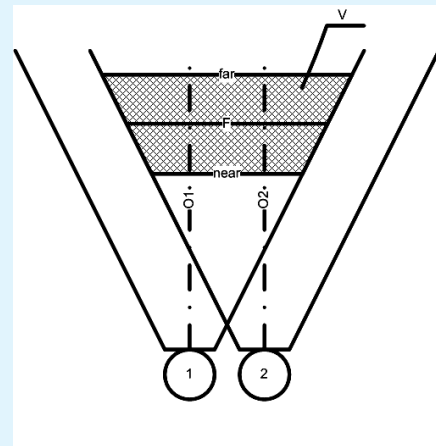


Figure 3b: An example of marker position registration method using two optical cameras.

### Computed Neurosurgery Planning System

The study method consists of two algorithms:

- Calculation of shortest surgical access to the target (invasive surgical access), which describes the risk of surgical access, which based on the distance from the end point of the trajectory, toward the stereotactic target point.
- And assuring the safety path by avoiding risk map, which would take into account the physiological significance details of each anatomical structure

through the track, the high density tissues such as bones (CT contrast data visualization).

### Invasive Surgical Access

To assess the specific surgical approach is necessary to formalize the parameters determining the risk of such access. This allows you to set a specific surgical approach in the corresponding to numerical value that specify the invasiveness value and type, as a result choose the least traumatic neuro surgical access.

Each element of the surgical access track  $(x(n), y(n), z(n))$  determined by the expression (1) based on the target coordinates  $(x_T, y_T, z_T)$ , and the intact coordinates  $(x_M, y_M, z_M)$ , and the step  $(\Delta t)$ .

$$\begin{cases} x(n) = x_T + (x_I - x_T)n \cdot \Delta t; \\ y(n) = y_T + (y_I - y_T)n \cdot \Delta t; \\ z(n) = z_T + (z_I - z_T)n \cdot \Delta t, \end{cases} \quad (1)$$

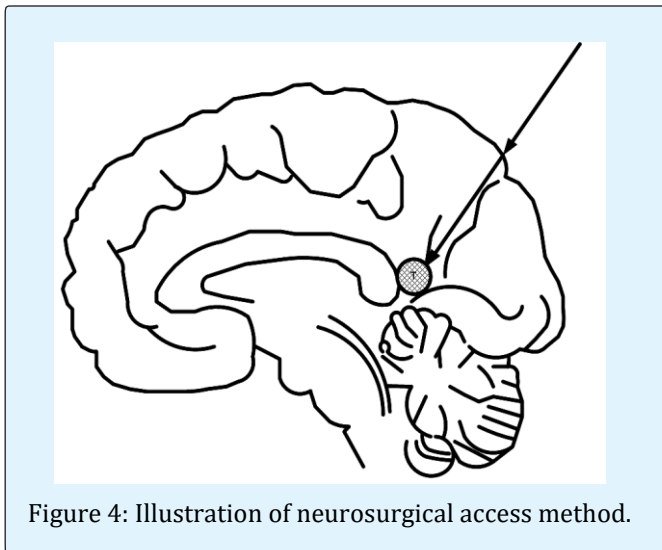


Figure 4: Illustration of neurosurgical access method.

### Computed Tomography Contrast Data Visualization System

For detailing of each anatomical structure through the surgical track, the high density tissues such as bones and so on...CT contrast data visualization method was implement. Three subsystems (Figure 5) were constructed in the main system of CT contrast data visualization, in order to solve the problem statement;

- 1) Subsystem for obtaining the initial data,
- 2) Subsystem for user interface,
- 3) Subsystem for data processing and displaying.

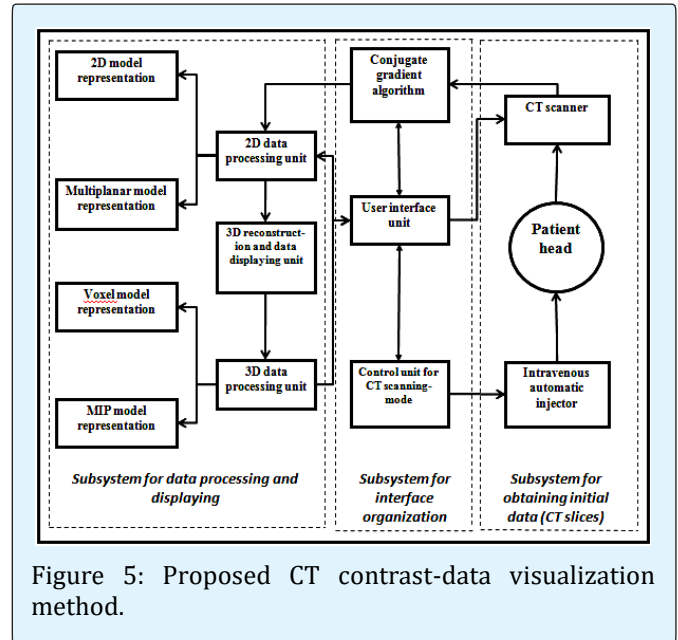


Figure 5: Proposed CT contrast-data visualization method.

The initial data was collect to conduct the study; the dataset is axial CT- slices, obtained by install CT scanner (Somatom and Siemens). The study implemented according to contrast scanning protocol (Injector Medrad Vistron CT) parallel to the base of the skull with a standard patient lying. The aim of this visualization protocol is to generate the best diagnostic data display and to illustrate the characteristic features that could aid in further CT image analysis. Scanning procedure was made with 1 mm step between the slices. The spatial characteristics of the investigated area, that is calculated by  $(N)$ , and this number usually equal  $(N > 100 \text{ slices})$ . CT-image intensity is represented by  $F(i,j)$  function, and specified in raster size  $(I \times J)$ , by mean (an image size should be  $512 \times 512$  elements). The intensity image element calculate in pixel, and used for every CT slide with a coordinates of  $(i,j)$ , that is relatively equivalent to the attenuated X-rays passed the tissue at the volume unit, projected on a specified point..

The first subsystem consists of spiral CT scanner and automatic injection unit for intra vital stain injection, which is used according to the pre-mentioned protocol (input data), that could be used for determination of the operation mode of the subsystem. CT imaging system starts scanning the study area after a short time interval of injection process. CT resulting images contain a set of slices, preliminary processed in CT calculation unit. These slices are then transmitted to conjugate gradient algorithm where the data are processed in the 2D module.

The interface organization subsystem consists of: 1) conjugate gradient algorithm for data obtaining and processing, 2) CT scanning-mode control unit, for specifying the data flow and volume parameters, as well as the duration of intra vital stain injection, and the delay time before starting scanning, 3) The user interface module for guarantying the interaction between the radiologist and imaging system (hard software) and linking the visualization software to the hardware.

The subsystem of data processing and visualization is based on a high speed-graphic station. It consists of: 1) Data-processing software (2D and 3D), which is used for formation of 3D model and data animation, 2) Data visualization unit in 2D and 3D modes. The algorithms of 2D data display carry out visualization of 2D and 2.5D models. Moreover, these subsystems responsible for reconstruction of the multi planar model. Volumetric data visualization is performed by Voxel visualization unit and the Maximum Intensity Projection (MIP) unit.

### The Implementation of 2D Data Processing and Algorithm for Data Visualization

2D data processing deals with some isolated slides located in individual multiplanar section. This type of processing is aimed at transformation of the initial data, in order to improve the visual monitoring of brain anatomical structure. Furthermore, image correction mode should be selected at this stage, allowing improvement of identification of brain vascular system location, as well as, performing the detection and identification of possible brain anomalies. The main algorithm of image processing at current stage is the local operations, related to the initial data transformation for defining images radio density, using the scale of Hounsfield HU (-1000÷1000 unit of HU), in intensity gradient of 256 intensity levels in the graphical data display system. The methods of intensity correction histogram are used to increase the brightness and contrast of displayed image. The median filtering algorithms were used to eliminate the local interference that could prevent image blurring, the same as its analogue standard algorithms of averaging filtration. Selection of median filter mode is adaptively performed with respect to the noise geometrical dimensions and vessels, so as not to remove small formation of the vascular system. After elimination of the local noise, it is necessary to perform high-frequency filtration of resulting images for further improvement of the displayed vascular system.

The obtained data after filtration is transferred to the unit of 2D visualization for immediate display. During this stage, the 2D visualization unit provides CT slices in the coordinate system and various measurement procedures for more diagnostic information.

Multipanar model reconstruction unit displays the structures of the model, slices located not parallel to the scanning plane. It is used to monitor vessels having a large branching degree and variability, as well as visually monitoring the orientation of the anatomical configuration. Algorithm of reconstruction of the multipanar model is based on reconstructing plane P by three points  $A(A_x, A_y, A_z)$ ,  $B(B_x, B_y, B_z)$  and  $C(C_x, C_y, C_z)$  as in Figure 6. Two points are usually defined by a single plane of the CT slice; the third point defines the orientation of the model at vertical plane. Moreover, the framework of the model is determined by upper and lower numbers of CT slice.

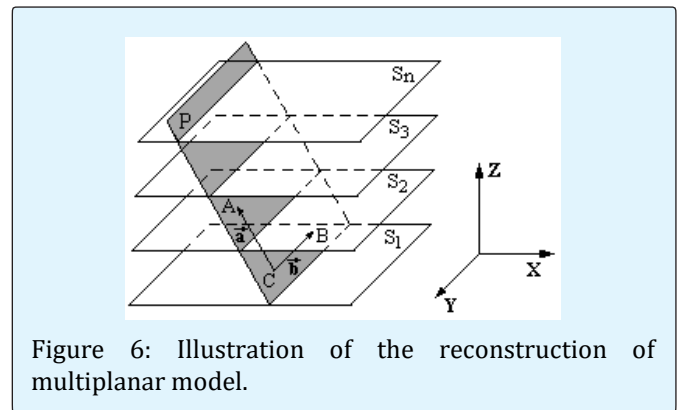


Figure 6: Illustration of the reconstruction of multipanar model.

In case of establishing the multipanar model perpendicular to the scanning plane, the third point is automatically specified, and its coordinates of (x, y) match with the coordinates of one points previously selected-coordinate is determined by the maximum/minimum slice number (Sn), used in reconstruction procedure. Thus, the model plane (figure 6) is parametrically determined by the equation:

$$P(t, s) = C + \vec{a}t + \vec{b}s = C + (\overrightarrow{A - C})t + (\overrightarrow{B - C})s, \quad (2)$$


Where t and s is parameters:  $t, s \in [0, 1]$ .

In coordinate form, the equation (1) was used for calculation of the plane:

$$P(t, s) = (C_x + a_x t + b_x s, C_y + a_y t + b_y s, C_z + a_z t + b_z s)$$

Elimination of polygons (tiled surface), associated with the smallest spatial structures in Z plane of the image, it is necessary to apply the procedure of low-

frequency filtration which clearly visualize vessels perpendicular to the scanning plane (Figure 7).

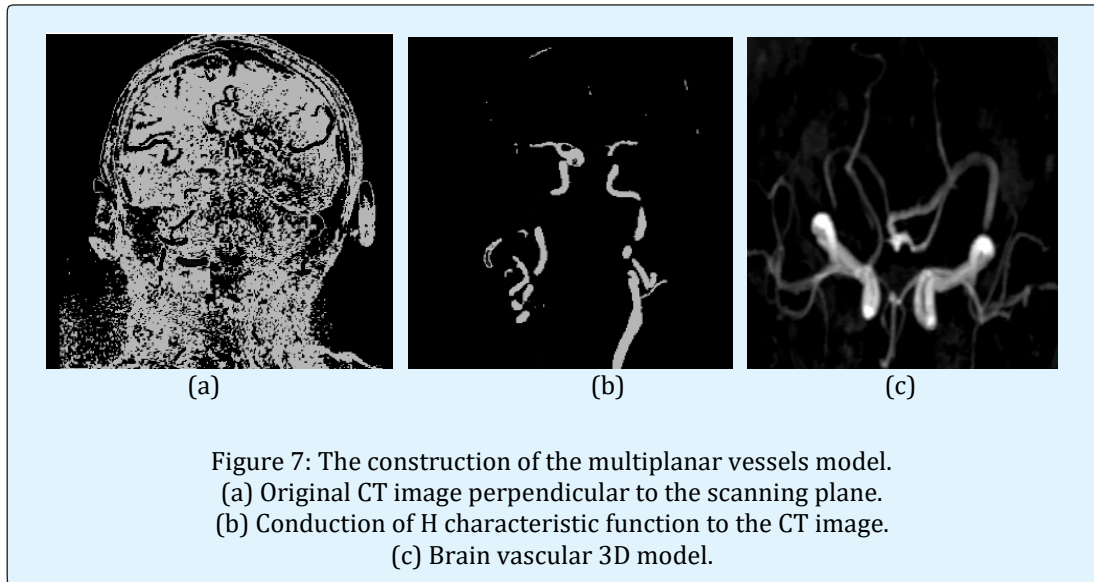


2.5D image contain detailed information about the anatomical structure. Therefore, special graphical buffers (G-buffers), containing additional information about the image, are used to construct the 2.5D image. The Basic components of 2.5D model are: characteristics buffer (H buffer) and identification buffer (ID buffer) (Figure 5). The control unit of displaying mode determines the data monitoring method when combining data buffers. The Original Image of CT slices are stored in (OI-buffer). 2.5D visualization mode performs selective isolation and pseudo coloring of different anatomical objects (Figure 8).


CT contrast-data stored in H-buffer contains information about the characteristic function (binary images) of vessels. This information is gained according to data describing the density of blood vessels that is filled with intra vital stain (contrast medium):

$$H(i, j) = \begin{cases} 0; & \text{at } F(i, j) < T_{\min}; \\ 1; & \text{at } T_{\min} \leq F(i, j) \leq T_{\max}; \\ 0; & \text{at } F(i, j) > T_{\max}, \end{cases} \quad (3)$$

Where  $T_{\min} \approx 100HU$  and  $T_{\max} \approx 300HU$  is the minimum and the maximum threshold values of the vascular channel density, respectively.

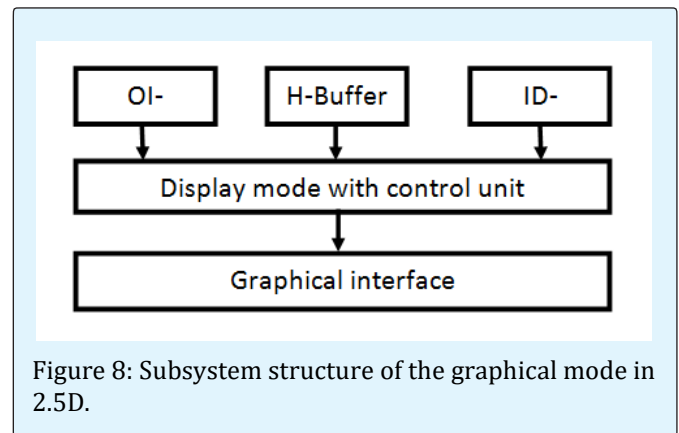

The original image and its corresponding content are stored in H-buffer (Figure 9a & 9b) to increase the visibility of image mapping provided with an inverse characteristic function  $H'(i, j) = 1 - H(i, j)$ .

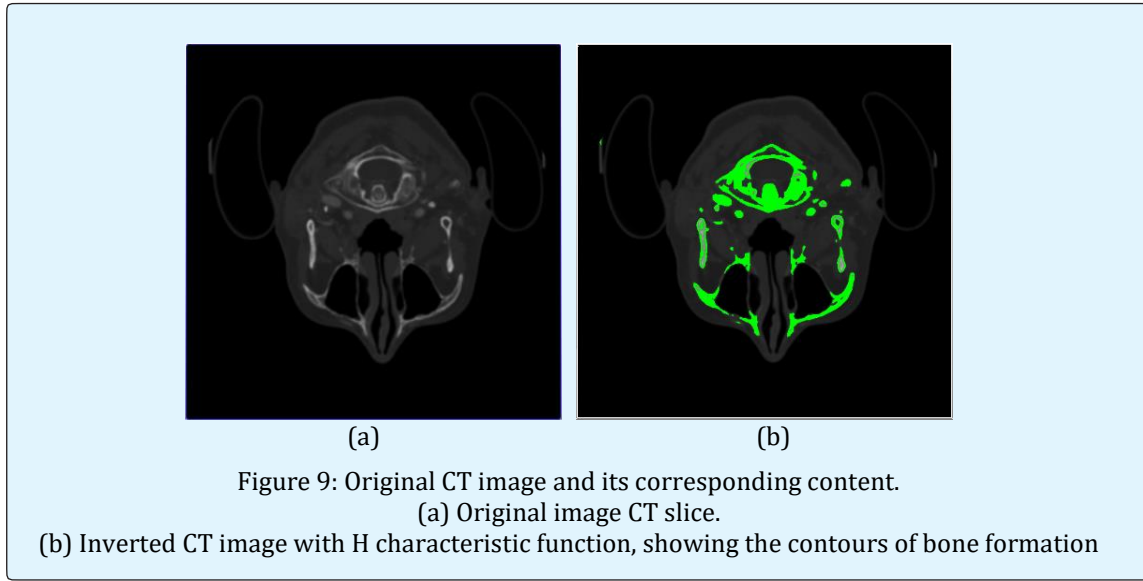


Logical filtering of the characteristic function values was performed to eliminate the local noises and false objects in H-buffer (for example, image elements that located at the bone medulla boundary).

ID buffer data, containing the individual identifiers of brain anatomical structures, is based on the methods of multi-value image segmentation, using sequential segmentation algorithms [10]. Initially, this algorithm is based on density differences, followed by geometric characteristics (size, shape, location, etc.). At this stage, minimum degree of automation is used, requiring further investigation.

### Implementation of 3D Processing Algorithm and Data Visualization

Three dimensional (3D) method of visualization CT-data is used for more accurate determination of localization and disease nature, as well as implementation of the surgical planning. The basic principle of CT-image formation of scan area is dividing the image into simple volumes, where each volume is characterized by a number of Hounsfield (Hu) and each of these volume parts is called volume element (voxel) as shown in (Figure 7a). Extraction efficiency of complex polygonal models requires for addition on processing system and module displaying tomographic data for polygons optimization. This optimization should include reducing the number of triangles, describing a display object by removing obviously invisible parts, combining several triangles lying in the same plane of one triangle. Thus,

when preparation voxel model, advisable to carry out the removal as individual faces, that common to multiple voxels, as well as elimination of whole voxels invisible from the outside of the model. Combining adjacent faces of voxels in one face spills in a significant reduction the number of primitives of the model. Rearranging flow vertex indices of triangles based on organization transformation cache video card, allow to reduces the number of performed transformation matrix and significantly increase the number of displayed triangle model per moment of time. Described above optimization techniques allow in real-time to model visualization, to obtained triangulation tomographic large amounts of data (hundreds of millions of voxels). However, in order to perform visualization of volumetric network data, need to know exactly which voxels from belong investigated object and must be displayed when rendering, and which are contrary discarded. This procedure is carried out by the formation of binary mask, obtained after first segmentation data imaging. The operation of selection the first brightness for visible items tomographic cube should be in the manual mode and require for an interactive original data of mapping when changing visible brightness range rendered voxels. To resolve this task, and to satisfy the mentioned requirements, by the method of discarding rays before first collision. It allows instantly to obtain highly voxel detailed projection studied objects. While dynamical changing first mapping. The results of applying this method to a sequence of tomography slices of the patient's head for different values of the first presentation in Figure 10b.

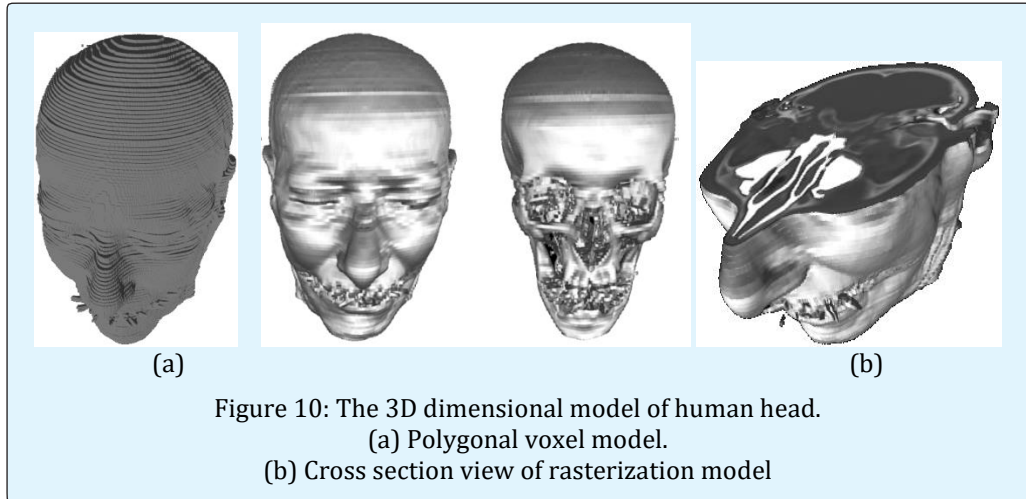

Collection of structured data is generated (structured data-set), representing an array of values describing the intensity function with coordinates of  $\{x_i, y_j, z_k\}$  [11,12]:

$$V_{ijk} = V(x_i, y_j, z_k), \dots\dots\dots (4)$$

Where

$$x_i = x_0 + i\Delta x,$$

$$y_j = y_0 + j\Delta y,$$


$$z_k = z_0 + k\Delta z.$$

Each  $V_{ijk}$  value can be considered as an average volume, in measurement field as a rectangle, parallel to planes  $\Delta x, \Delta y, \Delta z$ , whose center is located at point  $(x_i, y_j, z_k)$ . This simple rectangle defines the volume element.

3D visualization of CT contrast-data is implemented by 2 modes: 1) gray-scale voxel visualization method, and 2) display algorithm using maximum intensity projection (MIP).

In case of 3D voxel visualization, the object is represented as a set of voxels. The 3D model is performed using 3D raster visualization. The additional characteristic of voxel is that it expresses the transparency degree. This visualization can be carried out using partial slices through alteration of the transparency degree of voxels for different objects; taking into account of the transparent voxel objects should be removed. Current visualization method could estimate the spatial relationships between the vessels and surrounding structures (Figure 11a).

When utilizing the (MIP) algorithm method of visualization, display band of intensity levels is selected and construction of display list containing voxel with intensity in a given interval (Figure 11b). The main difficulty of this mode is manifestation of structures having a similar intensity, but it could simultaneously represent anatomical objects of different nature (for example, intravital-stained vessels and fine bone structures).

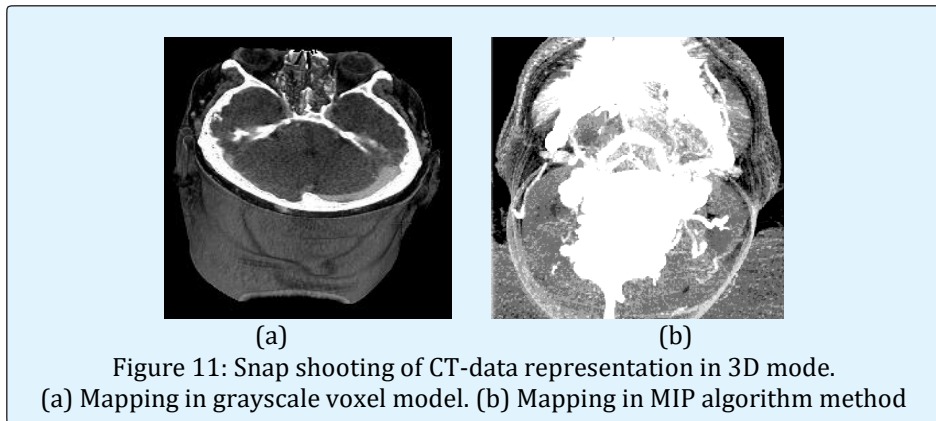

**Results**

It will be appreciated that the stereotactic access is direct access to the target in three-dimensional space (figure12). In this same study, as illustrations will use the two-dimensional scheme in order to increase the visibility of the material land improve its perception. Accordingly, the surgical access in the one plane, sure it will show the target and the access angle better.

Consider a variety of methods of determinations the invasiveness of surgical approach.


The simplest method is “2” which describes the risk of surgical access (RE), which expressed by the distance from the endpoint of the trajectory (intact - T), toward the stereotactic target point (I).

$$R_E = \sqrt{(T_x - I_x)^2 + (T_y - I_y)^2}$$

$$R_E = \sqrt{(T_x - I_x)^2 + (T_y - I_y)^2} \quad (5)$$

Figure 12 shows the risk evolution of the surgical procedure done by (5), 24 accesses, and the smaller the risk, the darker it is represented in the geometric anatomical graph (Figure 12a).

Normalized values of risk are shown in Figure 10b (square of the distance and the distance). Thus, the method to determine the risk of surgery values is not taking into the account of the anatomical features of the human brain, and therefore it cannot be used in actual systems neuro-surgical planning.

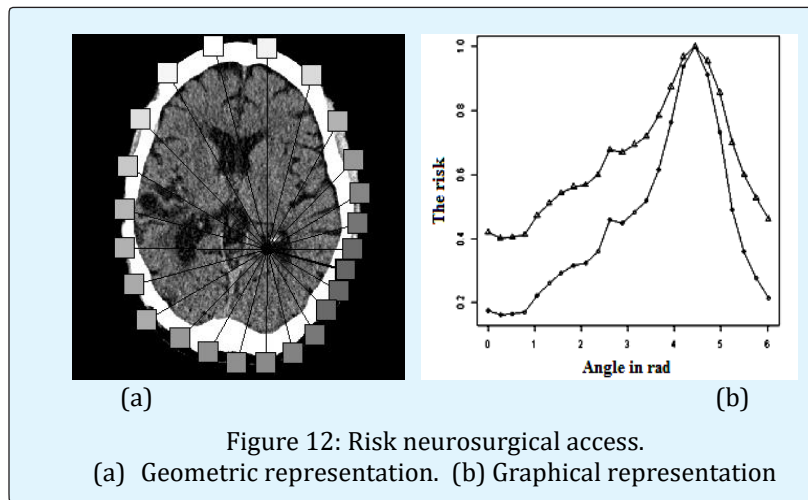

It is therefore necessary to include personal volumetric map for the invasiveness track, which would take into account the physiological significance details of

each anatomical structure through the track, as well as the value of the risk of the surgical access [20].


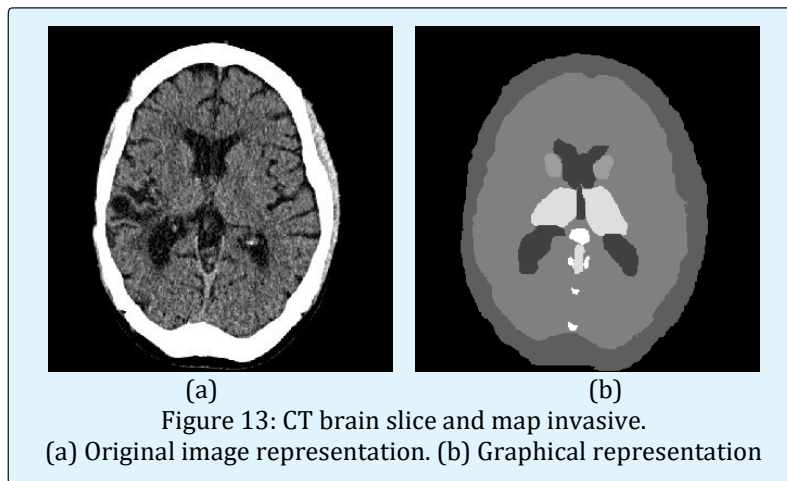


Figure 13 shows an example of the CT slice of the human brain and its corresponding graphical image assigned the invasiveness (the lighter structures in the slice, the higher risk during the surgery). It will be appreciated that will use of additional CT study as a geography, allows to expand and improve considerably invasiveness map. This is primarily due to the large value important that will give to the index contain blood vessels [25].

Using of invasiveness map, allows of the access risk (RA) evaluation, by the sum of the index values (ID) which located along the investigational surgical track (6).

$$R_A = \sum_{i=1}^N ID_i \quad (6)$$

Figure 5 shows an example of the calculation of neurosurgical access done by (5) and (6) together. As can be seen from Figure 14b, in the approach referred o (6), there are additional minima that correspond to the optimal track in this slice. With decreasing of the angle step that specifies the surgical access, the accuracy will increase, and will found a new track that is located near hazardous anatomical structures (data for a high-risk surgical procedure).

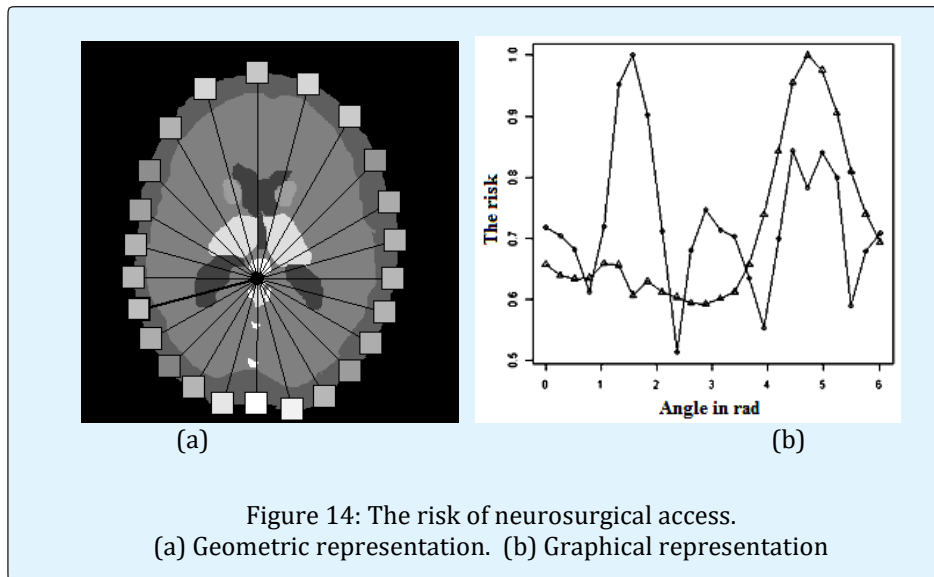

### Conclusion and Future Work

The study reached the following conclusions:

- The (Risk Map) of brain structures is an effective approach to the definition of the risk of surgical approach.
- The choice of surgical approach should take into account the geometry of the surgical instrument track, as well as the errors of the stereotactic navigation system;
- The accuracy of the navigation system must be much higher than to make the decision of surgery depending on the simulation systems only (Interactive with the user);
- The choice of surgical approach should take into account the possible brain structures displacement, in accordance with the type of trepanation.
- A promising direction for further researching this area is the implementation of these descriptive approaches

in a computer system planning neurosurgery. It is also necessary to determine the optimal surgical approaches, taking into account which will allow determining the trajectory, including a minimum with broad flat areas.

- The significance of the current study also relies in the advances of computer aided design applications for obtaining and displaying more diagnostic information to be used in neurosurgical planning systems. Increasing of data obtaining and diagnostic significance, using the method of CT contrast-data, can be achieved via developing and improving data visualization algorithms. Therefore, one of the main parts of the CT contrast-data visualization system is the subsystem of secondary processing data and display unit.
- The display methods of the vascular system data, using CT contrast-data, are divided into 2D and 3D models. The first algorithm has a relatively low visibility, but

allows accurate measurements of the anatomical-structure parameters. The most effective method of 2D visualization is the display mode in 2.5D associated with using structures containing more data about the anatomical objects. The 3D model is designed for virtual examination of spatial relationships between anatomical structures as well as 3D visualization of the vascular channel.

- Our current algorithms develop appropriate software allowing a proper visualization the vascular system of the brain in different modes with scanning increments of 1 mm, confirmed via testing the results of the work in the diagnostic center of Kharkov regional clinical hospital. The significance of the current research is the development of algorithms for automatic identification of vascular system, obtaining and displaying more diagnostic data of neurosurgical planning systems.
- finally, ratification: all the functions of selecting surgical access is observed and completely controlled by the user

### Conflicts of Interest

O. G. Avrunin, Husham Farouk Ismail Saied, are declare that they have no conflict of interest.

**Ethical standards:** All procedures performed in studies involving human participants were in accordance with the ethical standards of the institutional and/or national research committee and with the 1964 Declaration of Helsinki and its later amendments or comparable ethical standards.

**Informed consent:** For a retrospective study of anonymized image data, informed consent is not required.

### Acknowledgement

The authors extend their appreciation to the College of Applied Medical Sciences Research Center and the Deanship of Scientific Research Prince at Sattam Bin Abdulaziz University for funding this research.

### References

1. Smith-Bindman R, Lipson J, Marcus R, Kim KP, Mahesh M, et al. (December 2009) Radiation dose associated with common computed tomography examinations and the associated lifetime attributable risk of cancer. *Arch Intern Med* 169(22): 2078-2086.
2. Galloway RL (2015) Introduction and Historical Perspectives on Image-Guided Surgery. In Golby, AJ. *Image-Guided Neurosurgery*. Amsterdam: Elsevier, pp: 1-22.
3. Tse VCK, Kalani MYS, Adler JR (2015) Techniques of Stereotactic Localization. In Chin, LS; Regine, WF. *Principles and Practice of Stereotactic Radiosurgery*. Springer, New York, pp: 25-32.
4. Agarwal J, Munshi A, Rathod S (2012) Skin markings methods and guidelines: A reality in image guidance radiotherapy era. *South Asian Journal of Cancer* 1(1): 27-29.
5. Eggebrecht AT, White BR, Ferradal SL, Chen C, Zhan Y, et al. (2012) A quantitative spatial comparison of high-density diffuse optical tomography and fMRI cortical mapping. *Neuroimage* 61(4): 1120-1128.
6. Carlson Neil R (2013) *Physiology of Behavior*. Pearson Education Inc., pp: 134.
7. Wintermark M, Fischbein NJ, Smith WS, Ko NU, Quist M, et al. (2005) Accuracy of dynamic perfusion CT with de convolution in detecting acute hemispheric stroke. *AJNR Am J Neuroradiol* 26(1): 104-112.
8. Barnett GH, Linskey ME, Adler JR, Cozzens JW, Friedman WA, et al. (2007) Stereotactic radiosurgery- an organized neurosurgery-sanctioned definition. *Journal of Neurosurgery* 106(1): 1-5.
9. Tsao May N, Rades D, Wirth A, Lo SS, Danielson BL, et al. (2012) International Practice Survey on the Management of Brain Metastases: Third International Consensus Workshop on Palliative Radiotherapy and Symptom Control. *Clinical Oncology* 24 (6): e81-e92.
10. Park Kyung-Jae, Kondziolka D, Kano H, Berkowitz O, Ahmed SF, et al. (2012) Outcomes of Gamma Knife surgery for trigeminal neuralgia secondary to vertebrobasilar ectasia. *Journal of Neurosurgery*. 116(1): 73-81.
11. Adler JR (2013) The future of robotics in radiosurgery. *Neurosurgery* 72(S1): 8-11.
12. Leclerc X, Taschner CA, Vidal A, Strecker G, Savage J, et al. (2006) The role of spiral CT for the assessment of the intracranial circulation in suspected brain-death. *J Neuroradiol T* 33(2): 90-95.
13. Wurm RE, Erbel S, Schwenkert I, Gum F, Agaoglu D, et al. (2008) Novalis Radiosurgery frameless image-

- guided noninvasive radiosurgery: initial experience. *Neurosurgery* 62 (5): A11-A18.
14. Lars Muckli, Marcus J Naumer, Wolf Singer (2009) Bilateral visual field maps in a patient with only one hemisphere. *PNAS Organization* 106 (31): 13034-13039.
  15. Rozumenko VD, Chuvashova OY, Ruditsa VI, Artem R (2011) MR-tractography in image-guided surgery of brain tumors. *Ukrainian Neurosurgical Journal* 2: 65-69.
  16. Howick J, Cohen BA, McCulloch P, Thompson M, Skinner SA (2015) Foundations for evidence-based intraoperative neurophysiological monitoring. *Clin Neurophysiol* 127(1): 81-90.
  17. Nuwer MR (2015) Measuring outcomes for neurophysiological intraoperative monitoring. *Clin Neurophys* 127(1): 3-4.
  18. Herman GT (2009) *Fundamentals of computerized tomography: Image reconstruction from projection*, 2<sup>nd</sup> (Edn.), Springer.
  19. Martin CM, Charlotte DB, Miriam U, Julia S, Dilworth YP, et al. (2013) 3D spectral imaging with synchrotron Fourier transforms infrared spectro-microtomography. *Nature Methods* 10: 861-864.
  20. Mojtaba Ahadi, Maryam Isa, Iqbal Saripan M, Hasan WZW (2015) Three dimensions localization of tumors in confocal microwave imaging for breast cancer detection. *Microwave and Optical Technology Letters* 57(12): 2917-2929.
  21. Brunenberg E JL, Vilanova A, Visser-Vandewalle V, Temel Y, Ackermans L, et al. (2007) Automatic Trajectory Planning for Deep Brain Stimulation: A Feasibility Study. In: Ayache N, Ourselin S, Maeder A, (Eds.), *Medical Image Computing and Computer-Assisted Intervention* 4791: 584-592.
  22. Shamir RR, Tamir I, Dabool E, Joskowicz L, Shoshan Y (2010) A method for planning safe trajectories in image-guided keyhole neurosurgery. *Med Image Comput Assist Interv* 13(3): 457-464.
  23. Avrunin OG, Alkhorayef M, Husham Farouk Ismail Saied, Tymkovych MY (2015) The Surgical Navigation System with Optical Position Determination Technology and Sources of Errors. *Journal of Medical Imaging and Health Informatics, American Scientific Publishers* 5(4): 1-8.
  24. Tymkovich MY (2012) Optical method for detecting the spatial position of the surgical instrument in a computer navigation system J. *Journal of National Technical University Kharkov Polytechnic Institute* 18: 124
  25. Rozumenko VD, Rozumenko AV (2010) Multimodal neuronavigation using in surgery of brain tumors. *Ukrainian Neurosurgical Journal* 4: 51-57.

