

Головний редактор:

П.І. Несажмаков, д-р техн. наук, проф., ННЦ “Інститут метрології”, Україна

Заступник головного редактора, науковий редактор:

Ю.Ф. Павленко, д-р техн. наук, проф., ННЦ “Інститут метрології”, Україна

Редакційна колегія:

О. Боднар, доц., університет Еребру, Швеція
О.М. Величко, д-р техн. наук, проф., ДП “Укрметртест-стандарт”, Україна
М.М. Горобець, д-р фіз.-мат. наук, проф., ХНУ імені В.Н. Каразіна, Україна
О.В. Дзисюк, Метрологічний центр військових еталонів Збройних Сил України, Україна
І.П. Захаров, д-р техн. наук, проф., ХНУРЕ, Україна
С.І. Кондрашов, д-р техн. наук, проф., НТУ “ХПІ”, Україна
О.Д. Купко, д-р техн. наук, ННЦ “Інститут метрології”, Україна
Е. Манске, д-р техн. наук, проф., Технічний університет Ільменау, Німеччина
Г. Мачін, д-р природничих наук, проф., Національна фізична лабораторія, Велика Британія
І.О. Мель, ННЦ “Інститут метрології”, Україна
Л.А. Назаренко, д-р техн. наук, проф., ХНУМГ ім. О.М. Бекетова, Україна
Г.Ю. Народницький, д-р техн. наук, ННЦ “Інститут метрології”, Україна
В.В. Паракуда, канд. техн. наук, доц., ДП “НДІ Система”, Україна
О.В. Прокопов, д-р фіз.-мат. наук, проф., ННЦ “Інститут метрології”, Україна
В.В. Семенець, д-р техн. наук, проф., ХНУРЕ, Україна
В.В. Склярів, канд. техн. наук, ННЦ “Інститут метрології”, Україна
Б.І. Стадник, д-р техн. наук, проф., НУ “Львівська політехніка”, Україна
Ю.М. Туз, д-р техн. наук, проф., НТУУ “КПІ ім. Ігоря Сікорського”, Україна

Відповідальний редактор С.В. Білоусова
Літературний редактор Н.О. Мірошніченко
Комп’ютерна верстка і дизайн Г.С. Мицик

Надруковано в ННЦ “Інститут метрології”.

Адреса редакції: ННЦ “Інститут метрології”,
вул. Мירוносицька, 42, м. Харків, 61002
Тел.: (057) 704-98-43, факс: (057) 700-34-47
E-mail: journal@metrology.kharkov.ua
Вебсайт: <http://umj.metrology.kharkov.ua/>

Видання індексується міжнародною бібліометричною та наукометричною базою даних **Web of Science Core Collection, Google Scholar, WorldCat і BASE**.
ISSN (Print) 2306-7039
ISSN (Online) 2522-1345
DOI: 10.24027/2306-7039

Журнал зареєстрований у Міністерстві юстиції України. Свідоцтво про державну реєстрацію серія КВ № 22932-12832ПР від 26 вересня 2017 р.
“Український метрологічний журнал” включено до Переліку наукових фахових видань України на підставі Наказу МОН України від 15 жовтня 2019 р. № 1301 (категорія “А”).
ННЦ “Інститут метрології” зареєстрований у Державному комітеті телебачення і радіомовлення України. Свідоцтво видавця серія ДК № 5944 від 15.01.2018 р.

Електронна версія – на сайті НБУ ім. В.І. Вернадського НАН України www.nbuv.gov.ua/portal/natural/Umlzh/index.html

Журнал видається з 1995 р.

Editor-in-Chief:

P. Neyezhmakov, National Scientific Centre “Institute of Metrology”, Kharkiv, Ukraine

Deputy Editor-in-Chief, Scientific Editor:

Yu. Pavlenko, National Scientific Centre “Institute of Metrology”, Kharkiv, Ukraine

Editorial Board:

O. Bodnar, Örebro University, Örebro, Sweden
O. Dzysyuk, Metrology Center of Military Standards of the Armed Forces of Ukraine, Kharkiv, Ukraine
M. Gorobets, V.N. Karazin Kharkiv National University, Kharkiv, Ukraine
S. Kondrashov, National Technical University “Kharkiv Polytechnic Institute”, Kharkiv, Ukraine
O. Kupko, National Scientific Centre “Institute of Metrology”, Kharkiv, Ukraine
G. Machin, National Physical Laboratory, Teddington, UK
E. Manske, Technical University of Ilmenau, Germany
I. Mel, National Scientific Centre “Institute of Metrology”, Kharkiv, Ukraine
G. Narodnytskyi, National Scientific Centre “Institute of Metrology”, Kharkiv, Ukraine
L. Nazarenko, O.M. Beketov National University of Urban Economy in Kharkiv, Kharkiv, Ukraine
V. Parakuda, DP NDI “Systema”, Lviv, Ukraine
O. Prokopov, National Scientific Centre “Institute of Metrology”, Kharkiv, Ukraine
V. Semenets, Kharkiv National University of Radio Electronics, Kharkiv, Ukraine
V. Sklyarov, National Scientific Centre “Institute of Metrology”, Kharkiv, Ukraine
B. Stadnyk, Lviv Polytechnic National University, Lviv, Ukraine
Yu. Tuz, National Technical University of Ukraine “Igor Sikorsky Kyiv Polytechnic Institute”, Kyiv, Ukraine
O. Velychko, SE “Ukrmetrteststandard”, Kyiv, Ukraine
I. Zakharov, Kharkiv National University of Radio Electronics, Kharkiv, Ukraine

Responsible Secretary S. Bilousova
Literary Editor N. Myroshnychenko
Desktop Publishing and Design A. Mytsik

The Journal is registered in the Ministry of Justice of Ukraine.

Editorial Address: NSC “Institute of Metrology”, Myronosytska Str., 42, Kharkiv, 61002
Tel.: (057) 704-98-43, fax: (057) 700-34-47
E-mail: journal@metrology.kharkov.ua
Website: <http://umj.metrology.kharkov.ua/>

The edition is indexed by international bibliometric and scientometric database: **Web of Science Core Collection, Google Scholar, WorldCat and BASE**.
ISSN (Print) 2306-7039
ISSN (Online) 2522-1345
DOI: 10.24027/2306-7039

The Certificate of State Registration: series KV No. 22932-12832PR of September 26, 2017.
“Ukrainian Metrological Journal” was included to the List of scientific specialized editions of Ukraine based on the Order of the Ministry of Education and Science of Ukraine No. 1301, dated October, 15, 2019 in category “A”.
NSC “Institute of Metrology” is registered in the State Committee for Television and Radio Broadcasting of Ukraine Certificate of publisher series DK No. 5944, dated January 15, 2018.

Electronic version is on the website of Vernadsky National Library of The NAS of Ukraine www.nbuv.gov.ua/portal/natural/Umlzh/index.html

The Journal has been issued since 1995

Вимірювання електричних та магнітних величин

- В.Ф. Болух, О.І. Вінніченко, П.І. Нєсжмаков, А.В. Омельченко.* Зменшення автосейсмічних коливань балістичного лазерного гравіметра за рахунок збудження індукційно-динамічної катапульти пакетом імпульсів 3
- О.М. Величко, Т.Б. Гордієнко.* Основні результати додаткових звірень для електричної енергії GULFMET.EM-S5/5.1 на частотах 50/53 Гц..... 12
- М.Г. Кокодій, А.О. Натарова, С.В. Погорєлов.* Вимірювання характеристик захисних екранів мікрохвильового випромінювання, які використовують тонкі провідні волокна..... 20
- В.Я. Гальченко, А.В. Сторчак, Р.В. Трємбовецька, В.В. Тичков.* Створення сурогатної моделі для відновлення приповерхневих профілів електрофізичних характеристик циліндричних об'єктів 27

Вимірювання маси та пов'язаних із нею величин

- І.П. Захаров, О.А. Боцюра, О.М. Паценко.* Врахування ексцесів вхідних величин у процедурі оцінювання невизначеності вимірювань на прикладі калібрування гирі 36

Вимірювання температури та теплофізичних властивостей

- О.В. Заболотний, В.А. Заболотний, М.Д. Кошовий.* Первинний вимірювальний перетворювач вмісту вологи для контролю якості зерна 42
- В.Г. Васильєва, В.В. Шведова.* Аспекти визначення температурних градієнтів термостатичних камер..... 50

Фізико-хімічні вимірювання

- М. Вічарова, М. Розікова, Р. Палєнчар, І. Тєсарж.* Простежуваність до державних первинних еталонів у галузі фізичної хімії у СМІ 57

Геодезія та геоінформаційне моделювання

- К.А. Мамонов, Р.С. В'яткін, О.С. Камєнєв, В.І. Троян.* Математичне моделювання рівня використання земель об'єктів екомережі регіонів. 65

Інформація

- Оголошення про набір на курси підвищення кваліфікації фахівців 73



Measurements of electrical and magnetic quantities

- V. Bolyukh, O. Vinnichenko, P. Nyezhamkov, A. Omelchenko.* Reduction of auto seismic oscillations of the ballistic laser gravimeter on account of the excitation of the induction-dynamic catapult by a pulse packet. 3
- O. Velychko, T. Gordiyenko.* Main results of GULFMET.EM-S5/5.1 supplementary comparisons for electrical energy at frequencies of 50/53 Hz .. 12
- N. Kokodiy, A. Natarova, S. Pogorelov.* Measurement of the characteristics of protective screens for microwave radiation made of thin conductive fibers 20
- V. Halchenko, A. Storchak, R. Trembovetska, V. Tychkov.* The creation of a surrogate model for restoring surface profiles of the electrophysical characteristics of cylindrical objects 27



Measurements of mass and related quantities

- I. Zakharov, O. Botsiura, O. Patsenko.* Accounting for the kurtoses of input quantities in the procedure of evaluating measurement uncertainty using the example of weight calibration 36



Measurements of temperature and thermophysical properties

- O. Zabolotnyi, V. Zabolotnyi, N. Koshevoy.* Primary measuring transducer of moisture content for grain quality control..... 42
- V. Vasylieva, V. Shvedova.* The aspects of determining the temperature gradients of thermostatic chambers 50



Physical and chemical measurements

- M. Vičarová, M. Roziková, R. Palenčár, J. Tesař.* The physical chemistry primary traceability at CMI 57



Geodesy and geoinformation modeling

- K. Mamonov, R. Viatkin, O. Kamieniev, V. Troian.* Mathematical modeling of the level of land use of the objects of the ecological network of regions. 65



Information

- Announcement of the intake to the courses of advanced training of specialists 73



Reduction of auto seismic oscillations of the ballistic laser gravimeter on account of the excitation of the induction-dynamic catapult by a pulse packet

V. Bolyukh¹, O. Vinnichenko², P. Neyezhnikov², A. Omelchenko³

¹ National Technical University "Kharkiv Polytechnic Institute", Kyrpychova Str., 2, 61002, Kharkiv, Ukraine
vfbolyukh@gmail.com

² National Scientific Centre "Institute of Metrology", Myronosytska Str., 42, 61002, Kharkiv, Ukraine
vinnsc2@gmail.com

³ Kharkiv National University of Radio Electronics, Nauky Ave., 14, 61166, Kharkiv, Ukraine
omela5656@gmail.com

Abstract

In order to reduce auto seismic oscillations in the ballistic laser gravimeters (BLG) with a symmetric method of measuring the gravitational acceleration (GA), an induction-dynamic catapult (IDC) is used, which is excited by a pulse packet from a capacitive energy storage unit (CES). With such excitation, a decrease in the amplitude of auto seismic oscillations is achieved by reducing the amplitude and increasing the duration of action of the electrodynamic force that occurs in the IDC when pushing the test body (TB).

A mathematical model of the IDC of the ballistic laser gravimeter with a symmetric method of measuring the GA is developed and the modeling of its electromechanical characteristics is carried out. Various methods of generating a packet of excitation pulses of the IDC inductor are considered and the characteristics of electrodynamic force pulses that accelerate the armature of the catapult with TB are investigated for them. The effect of IDC excitation by a pulse packet on the auto seismic component of the GA measurement is investigated. It is shown that on account of the excitation of the IDC by a ten-pulse packet, the auto seismic component of the uncertainty of the GA measurement by ballistic gravimeters can be reduced several (3–5) times in comparison with the excitation of the catapult by a single pulse.

Keywords: ballistic laser gravimeter; induction-dynamic catapult; auto seismic component of measurement uncertainty.

Received: 06.07.2020

Edited: 24.07.2020

Approved for publication: 31.07.2020

Introduction

For high-precision measurements of the absolute value of the gravitational acceleration g , the ballistic laser gravimeters (BLG) are used, in which a test body (TB) is pushed, which is an integral part of the Michelson laser interferometer measuring system [1–4]. The BLG measures the path and time intervals of the TB during its free movement in the vacuum chamber of the gravimeter [1]. Two types of gravimeters with free movement of the TB in a gravitational field are used, which implement symmetric and asymmetric methods of measuring g . In the symmetric method, the measurement of g is performed on both the upward and downward branches of the TB trajectory, and in the asymmetric method – only on the downward one. BLGs with a symmetric measurement scheme have a number of advantages. Since the resistance forces of the gaseous medium affect the measurement result with

opposite signs during the rise and fall of the TB, there is a mutual compensation. In addition, there is no problem of raising the TB to the starting position, as in a gravimeter with an asymmetric measurement scheme [5, 6]. The main disadvantage of a BLG with a symmetrical measurement scheme of g is the mechanical impact that acts when pushing the TB by catapult. At this, auto seismic oscillations of the foundation and all mechanical elements of the gravimeter occur, which cause the corresponding component of the measurement uncertainty g [7, 8].

Analysis of literature data and problem statement

In a BLG with electromagnetic catapult, the indirect conversion of the CES electrical energy into vertical pushing of the TB is performed [6]. The pushing device is made on the basis of a symmetrical six-bar lever mechanism (pantograph) with a central axis fixed

in the vacuum chamber of the ballistic unit. The central axis is connected to the ferromagnetic armature of the catapult. When the electromagnet winding is excited by CES, a current pulse occurs and due to the magnetic field, a massive ferromagnetic armature is drawn into the inner cavity. Moving vertically down, the ferromagnetic armature pulls the pantograph, which by increasing the axial dimensions pushes the carriage with the TB vertically upward with subsequent capture.

This multi-stage conversion of the CES electrical energy into mechanical energy of the TB vertical motion is accompanied by friction and subsequent wear of the contacts of moving elements, vibration and shock in the connecting elements, damping of the part of energy, bending and deformation processes, etc.

In order to eliminate these components of the measurement uncertainty, it is proposed to use a BLG with an induction-dynamic catapult (IDC), which provides direct electromechanical energy conversion and allows to adjust easily the height of the TB pushing [9].

When the CES discharges on the inductor winding (IW), there is a current pulse, under the action of which the magnetic field directs current in the conductive armature (CA). Under the action of axial electrodynamic force (EDF) f_z , the repulsion of the CA together with the TB performs free vertical movement ΔZ . At this, the receiving and emitting device activates and the measurement of g is performed. The short and significant amplitude EDF pulse between the IW and the CA of the catapult causes significant auto seismic oscillations of the BLG foundation, which affect the measurement of g . These oscillations can be reduced by increasing the duration and reducing the amplitude of the EDF between the IW and the CA by creating a packet of short power pulses of reduced amplitudes. The duration of the packet is determined by the period of propagation of the pulses generated at the excitation of the IDC from the CES sections.

The purpose of the study

The purpose of the study is to analyze the effect of the parameters of the excitation pulse packet of the IDC inductor on the EDF characteristics, which determine the magnitude of the auto seismic component of the uncertainty of the GA measurement.

Mathematical model of the BLG catapult

Let's consider the main processes in the IDC, which pushes the TB vertically upward. To solve this problem we use an approach based on the calculation of interconnected electromagnetic and mechanical processes [10].

In the catapult under consideration, when the IW with inductance L_1 and active resistance R_1 is connected to the CES, a current i_1 flows, which generates a magnetic field that induces current i_2 in the CA with inductance L_2 and active resistance R_2 . On

the account of EDF, the CA is pushed along the z axis with a speed v_z .

Initial conditions of the mathematical model:

$i_n(0) = 0$ – the current of the n -th element (1 – IW, 2 – CA);

$h_z(0) = 1 \text{ mm}$ – the initial axial shift of n -th elements;

$u(0) = U_0$ – the CES voltage with capacitance C_0 ;

$v_z(0) = 0$ – the velocity of the CA with the TB.

The solution of equations describing electrical, magnetic and mechanical processes is given in recurrent form [10]. Electrical processes in the IDC active elements are described by a system of equations [11]:

$$R_1 i_1 + L_1 \frac{di_1}{dt} + \frac{1}{C_0} \int_0^t i_1 dt + M_{12}(z) \frac{di_2}{dt} + v_z(t) i_2 \frac{dM_{12}}{dz} = 0, \quad \frac{1}{C_0} \int_0^t i_1 dt = U_0, \quad (1)$$

$$R_2 i_2 + L_2 \frac{di_2}{dt} + M_{21}(z) \frac{di_1}{dt} + i_1 v_z(t) \frac{dM_{21}}{dz} = 0, \quad (2)$$

where $M_{12} = M_{21}$ is the mutual inductance between the IW and the CA.

The system of equations (1)–(2) is reduced to the following equation:

$$a_3 \frac{d^3 i_1}{dt^3} + a_2 \frac{d^2 i_1}{dt^2} + a_1 \frac{di_1}{dt} + a_0 i_1 = 0, \quad (3)$$

where $a_3 = \nu$; $a_2 = \chi - 2Mv_z \frac{dM_{12}}{dz}$;

$$a_1 = R_1 R_2 + \frac{L_2}{C_0} - v_z^2 \left(\frac{dM_{12}}{dz} \right)^2; \quad a_0 = \frac{R_2}{C_0}; \quad \nu = L_1 L_2 - M_{12}^2;$$

$$\chi = R_1 L_2 + L_1 R_2.$$

The characteristic equation of differential equation (3) has the form [12]:

$$x^3 + r_* x^2 + s_* x + t_* = 0, \quad (4)$$

where $r_* = a_2/a_3$; $s_* = a_1/a_3$; $t_* = a_0/a_3$.

When substituting $y = x + r_*/3$, equation (4) is reduced to the form:

$$y^3 + p_* y + q_* = 0, \quad (5)$$

where $p_* = s_* - r_*^2/3$; $q_* = 2(r_*/3)^3 - r_* s_*/3 + t_*$.

The roots of equation (5) are found using the Cardano formula:

$$y_1 = u_* + v_*; \quad y_2 = \varepsilon_1 u_* + \varepsilon_2 v_*; \quad y_3 = \varepsilon_2 u_* + \varepsilon_1 v_*, \quad (6)$$

where $u_* = \sqrt[3]{D^{0.5} - 0.5q_*}$; $v_* = \sqrt[3]{-D^{0.5} - 0.5q_*}$;

$\varepsilon_{1,2} = 0.5(-1 \pm j\sqrt{3})$; $D = (p_*/3)^3 + (q_*/2)^2$ – discriminant of equation (5).

If $D < 0$, then after a series of transformations we obtain the expression for currents:

$$i_n(t_{k+1}) = \delta^{-1} \left\{ \left[i_n(t_k) - \frac{i_m(t_k)v_z^2}{R_1 R_2} \left(\frac{dM_{12}}{dz} \right)^2 \right] (\alpha_1 \beta_2 \beta_3 + \alpha_2 \beta_1 \beta_3 + \alpha_3 \beta_1 \beta_2) + \left(\Omega_n - \frac{v_z \Omega_m}{R_n} \frac{dM_{12}}{dz} \right) [\alpha_1 (\beta_2 + \beta_3) + \alpha_2 (\beta_1 + \beta_3) + \alpha_3 (\beta_1 + \beta_2)] + \left(\Lambda_n - \frac{v_z \Lambda_m}{R_n} \frac{dM_{12}}{dz} \right) (\alpha_1 + \alpha_2 + \alpha_3) \right\} \left[1 - \frac{v_z^2}{R_1 R_2} \left(\frac{dM_{12}}{dz} \right)^2 \right]^{-1}, \quad (7)$$

where $m = 1, 2$ at $n = 2, 1$;

$$\delta = \beta_1 \beta_2 (\beta_2 - \beta_1) + \beta_1 \beta_3 (\beta_1 - \beta_3) + \beta_2 \beta_3 (\beta_3 - \beta_2);$$

$$\Omega_n = B_n + \frac{B_m v_z}{R_n} \frac{dM_{12}}{dz}; \quad \Delta t = t_{k+1} - t_k; \quad \Lambda_n = E_n + \frac{E_m v_z}{R_n} \frac{dM_{12}}{dz};$$

$$\alpha_1 = (\beta_3 - \beta_2) \exp(\beta_1 \Delta t); \quad \alpha_2 = (\beta_1 - \beta_3) \exp(\beta_2 \Delta t); \quad \alpha_3 = (\beta_2 - \beta_1) \exp(\beta_3 \Delta t);$$

$$\beta_p = \left\{ 2(a_2^2 - 3a_1 a_3)^{0.5} \cos[2\pi(p-1)/3 + \varsigma] - a_2 \right\} / 3a_3;$$

$$\varsigma = \arccos \left[(a_2^2 - 3a_1 a_3)^{-1.5} (4, 5a_1 a_2 a_3 - a_2^3 - 13, 5a_0 a_3^2) \right]; \quad \gamma_1 = L_2; \quad \gamma_2 = -M_{12};$$

$$B_n = v^{-1} \left[i_n(t_k) \left(M_{12} v_z \frac{dM_{12}}{dz} - R_n L_m \right) + i_m(t_k) \left(R_m M_{12} - L_m v_z \frac{dM_{12}}{dz} \right) - \gamma_k u_c(t_k) \right];$$

$$E_1 = v^{-2} \left\{ i_1(t_k) \left[R_1 (R_2 M_{12}^2 + R_1 L_2^2 - C^{-1} L_2 v) - v_z M_{12} \frac{dM_{12}}{dz} (\chi + 2R_1 L_2) + v_z^2 (L_1 L_2 + M_{12}^2) \left(\frac{dM_{12}}{dz} \right)^2 \right] + i_2(t_k) \times \right. \\ \left. \times \left[v_z (L_2 \chi + 2R_2 M_{12}^2) \frac{dM_{12}}{dz} - M_{12} R_2 \chi - V^2 M_{12} L_2 \left(\frac{dM_{12}}{dz} \right)^2 \right] + u_c(t_k) \left(R_2 M_{12}^2 + L_2^2 R_1 - 2L_2 V M_{12} \frac{dM_{12}}{dz} \right) \right\};$$

$$E_2 = v^{-2} \left\{ i_1(t_k) \left[M_{12} (C^{-1} v - R_1 \chi) + v_z (2R_1 M_{12}^2 + L_1 \chi) \frac{dM_{12}}{dz} - 2v_z^2 L_1 M_{12} \left(\frac{dM_{12}}{dz} \right)^2 \right] + i_2(t_k) \left[R_2 (R_1 M_{12}^2 + R_2 L_1^2) - \right. \right. \\ \left. \left. - M_{12} v_z (2L_1 R_2 + \chi) \frac{dM_{12}}{dz} + (L_1 L_2 + M_{12}^2) v_z^2 \left(\frac{dM_{12}}{dz} \right)^2 \right] + u_c(t_k) \left[v_z (L_1 L_2 + M_{12}^2) \frac{dM_{12}}{dz} - M_{12} \chi \right] \right\},$$

where $u_c(t_k)$ is the CES voltage at the point of time t_k .

If the discriminant of the characteristic equation (5) $D > 0$, then after a series of transformations we obtain the expression for currents:

$$i_n(t_{k+1}) = \left(\xi_n - \frac{\xi_m v_z}{R_n} \frac{dM_{12}}{dz} \right) / \left[1 - \frac{v_z^2}{R_1 R_2} \left(\frac{dM_{12}}{dz} \right)^2 \right], \quad (8)$$

where

$$\xi_n = g^{-1} \left[g^2 + (f-d)^2 \right]^{-1} \left\{ g \cdot \exp(d\Delta t) \left[(g^2 + f^2) \Theta_n - 2f\Omega_n + \Lambda_n \right] + \exp(f\Delta t) \left\{ \sin(g\Delta t) d(f^2 - g^2 - fd) \Theta_n + \right. \right. \\ \left. \left. + (g^2 + d^2 - f^2) \Omega_n + (f-d) \Lambda_n \right\} + g \cdot \cos(g\Delta t) \left[d(d-2f) \Theta_n + 2f\Omega_n - \Lambda_n \right] \right\}; \quad \Theta_n = i_n(t_k) + \frac{v_z i_m(t_k)}{R_n} \frac{dM_{12}}{dz}.$$

Axial displacement of the armature with the TB occurs under the action of EDF:

$$f_z = i_1(t_k) i_2(t_k) \frac{dM_{12}}{dz}(z). \quad (9)$$

The value of the vertical displacement of the armature h_z can be given as a recurrent relation:

$$h_z(t_{k+1}) = h_z(t_k) + v_z(t_k) \Delta t + \vartheta \cdot \Delta t^2 / (m_1 + m_2), \quad (10)$$

where $v_z(t_{k+1}) = v_z(t_k) + \vartheta \cdot \Delta t / (m_1 + m_2)$ is the armature

velocity; $\vartheta = i_1(t_k) i_2(t_k) \frac{dM_{12}}{dz}(z) - g(m_1 + m_2)$,

m_1, m_2 is the weight of the armature and the TB, respectively.

The inductance of the n -th active element can be determined through the vector potential of the magnetic field when it is divided into elementary calculated circuits [13]. The mutual inductance between the n -th and m -th elementary circuits is determined by the method of Taylor series expansion [14].

Electromechanical processes in IDC during excitation by a single pulse

Let's consider the IDC with the following parameters: outer diameter of active elements $D_{ex} = 100$ mm, their inner diameter $D_{in} = 10$ mm. The IW height $H_1 = 10$ mm, height of the copper CA $H_2 = 2$ mm, number of the IW turns $N_1 = 46$ of wound copper bus with a cross section $a \times b = 1.8 \times 4.8$ mm². The TB mass $m_2 = 80$ g. The IDC is excited from the CES by a single pulse or packet of pulses at which the pushing of the armature together with the TB on the maximum height $h_{zm} = 120 \dots 160$ mm is provided. The total mass pushed is 220 g.

When the IDC is excited by a single pulse, let's consider the variant No. 1 of the CES low capacitance and overvoltage ($C_0 = 100 \mu\text{F}$, $U_0 = 730$ V) and the variant No. 2 of the CES large capacitance and under-voltage ($C_0 = 675 \mu\text{F}$, $U_0 = 210$ V) (Fig. 1).

When using the CES with low capacity C_0 and high voltage U_0 (variant No. 1), the amplitude of the current density in the IW is $j_{1m} = 155.7$ A/mm² in 0.075 ms, and the amplitude of the current density in the CA is $j_{2m} = 501.9$ A/mm². There is the EDF between the IW and the CA, the amplitude of which is $f_{zm} = 5092.8$ N. This provides acceleration of the armature with the TB to a velocity $v_z = 1.77$ m/s in 0.2 ms and the height of their push $h_{zm} = 158$ mm.

When using the CES with large capacity C_0 and low voltage U_0 (variant No. 2), all electromechanical processes are more stretched in time and smaller in amplitude. The amplitude of the current density in the IW reaches the value $j_{1m} = 100.9$ A/mm² in 0.18 ms, and the amplitude of the current density in the armature $j_{2m} = 306.0$ A/mm². When using such excitation, the EDF acts between the IW and the armature, the amplitude of which reaches $f_{zm} = 1993$ N. This provides acceleration of the armature with the TB to a velocity $v_z = 1.13$ m/s in 0.2 ms and the maximum height of their push $h_{zm} = 156$ mm. When using the CES of both variants, after some time (after ~ 0.35 ms) the velocities of the

armature become almost the same, amounting to $v_z = 1.70 \dots 1.78$ m/s.

As the duration of the force interaction between the IW and the armature increases (variant No. 2), the amplitude of the EDF decreases, although it remains at a high level. We would like to admit that even in this variant, the duration of the force remains unacceptably short (0.4 ms).

Electromechanical processes in IDC during excitation of the IW by a pulse packet

Let's consider the effect of the duration, shape and amplitude of a packet of 10 short power pulses between the IW and the CA on the electromechanical processes in the IDC. The specified pulse packet is formed by connecting the CES sections to the IW with a time delay that determines the pulse period.

Fig. 2 shows the electromechanical characteristics of the IDC when excited by a pulse packet lasting 12 ms from the CES sections with the same parameters: $C_0 = 100 \mu\text{F}$, $U_0 = 320$ V. With this method of the IDC excitation, the current density amplitude in the IW j_{1m} is successively reduced from 68.8 A/mm² in the first pulse to 47.7 A/mm² in the tenth pulse.

A greater decrease in the amplitudes of the induced current density occurs in the armature j_{2m} : in the first pulse of the packet it is 222.1 A/mm², and in the tenth pulse – 84.9 A/mm². There is a consistent decrease in the amplitude of the EDF pulses f_{zm} : from 997.3 N in the first pulse to 101.5 N in the tenth pulse. During the action of the pulse packet (12 ms) the armature together with the TB receive a velocity $v_z = 1.59$ m/s and travel a distance $h_z = 13.7$ mm. This packet of pulses provides pushing the armature together with the TB to a height $h_{zm} = 140.7$ mm.

To reduce the amplitude of the EDF of the first pulse of the packet, let's consider the excitation of the IDC from the CES sections with different parameters C_0 and U_0 . Fig. 3 shows the electromechanical characteristics

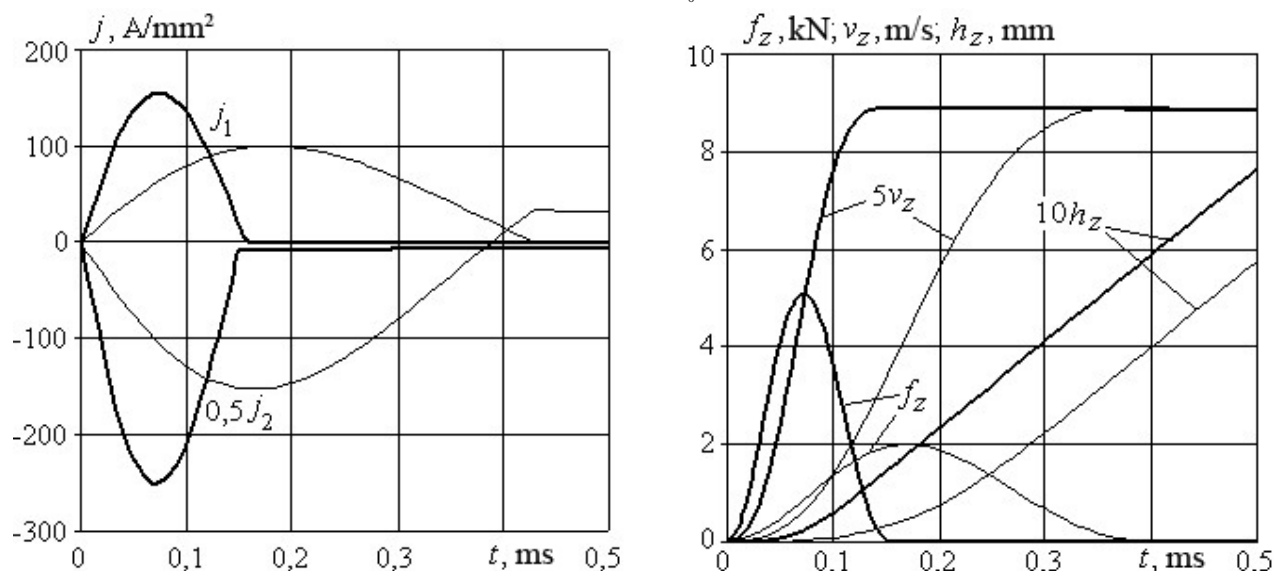


Fig. 1. Electromechanical characteristics of the IDC when excited by a single pulse: variant No. 1 of the CES (bold lines) and variant No. 2 of the CES (thin lines)


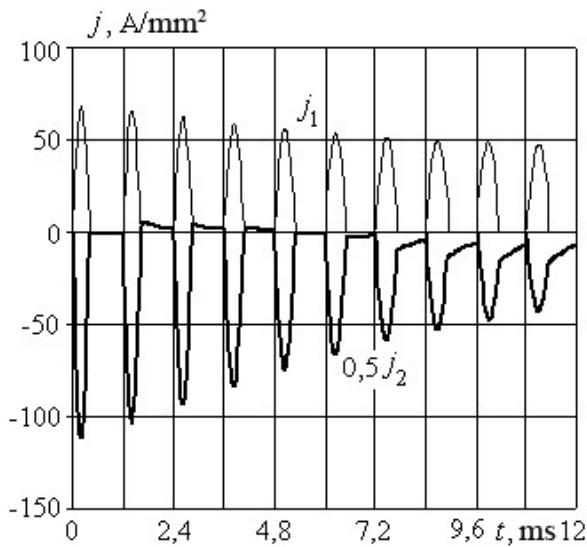


Fig. 2. Electromechanical characteristics of the IDC when excited by a packet of pulses from the CES sections with the same parameters: $C_0 = 100 \mu\text{F}$, $U_0 = 320 \text{ V}$

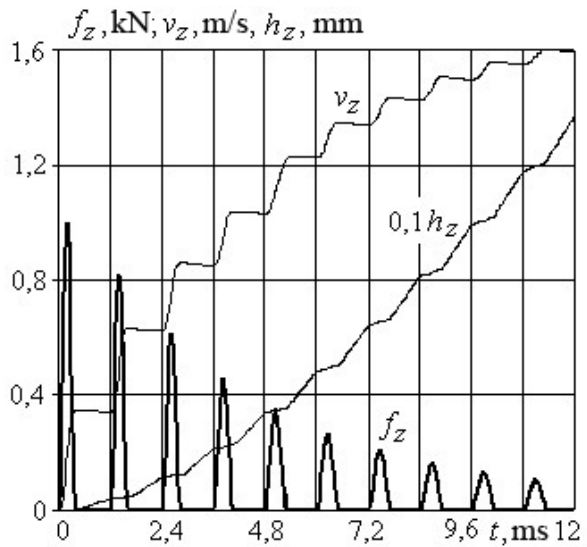

of the IDC when excited by a packet of pulses from the CES sections of the same capacitance $C_0 = 100 \mu\text{F}$, but charged to a voltage U_0 , which increases linearly from 150 to 420 V. With this excitation, the amplitude of the current density in the IW j_{1m} in all subsequent pulses of the packet gradually increases from 32.3 A/mm² in the first pulse to 67.3 A/mm² in the tenth pulse of the packet. The change in the amplitudes of the induced current density in the armature j_{2m} has the following pattern: in the first pulse, the amplitude is the smallest, 104.3 A/mm². In the following pulses, the amplitudes j_{2m} increase, reaching the highest value of 163.1 A/mm² in the seventh pulse, after which the amplitudes decrease to 150.8 A/mm² in the tenth pulse. In the first pulse, the amplitude of the EDF f_{zm} is the smallest, 218.5 N, then it increases, taking the largest value of 439.5 N in the fifth pulse, and then decreases. During the pulse packet, the armature together with the TB acquire a velocity $v_z = 1.48 \text{ m/s}$ and travel a distance $h_z = 8.5 \text{ mm}$. This packet of pulses provides pushing the armature to a height $h_{zm} = 132 \text{ mm}$.

Fig. 4 shows the electromechanical characteristics of the IDC when excited by a packet of pulses from the CES sections, charged to a voltage $U_0 = 210 \text{ V}$, which capacity C_0 increases linearly from 50 to 500 μF . The period between pulses is 3 ms. With this excitation, the amplitude of the current density in the IW j_{1m} in all subsequent pulses of the packet also gradually increases from 32.8 A/mm² in the first pulse to 64.5 A/mm² in the tenth pulse. The values of the amplitudes of the induced current density in the armature j_{2m} have the following pattern: in the first pulse the amplitude is the smallest, 107.2 A/mm², in subsequent pulses the amplitudes j_{2m} increase, reaching the highest value of 157.5 A/mm² in the fourth pulse, then decrease to 76 A/mm² in the tenth pulse.

At this, the amplitude of the EDF f_{zm} in the first pulse of the packet is 228.2 N, then it increases, taking the largest value of 465.6 N in the third pulse of the packet, and then decreases, taking the smallest value of 81.3 N in the tenth pulse. During the pulse packet (30 ms), the armature together with the TB acquire a velocity $v_z = 1.42 \text{ m/s}$ and moves a considerable distance

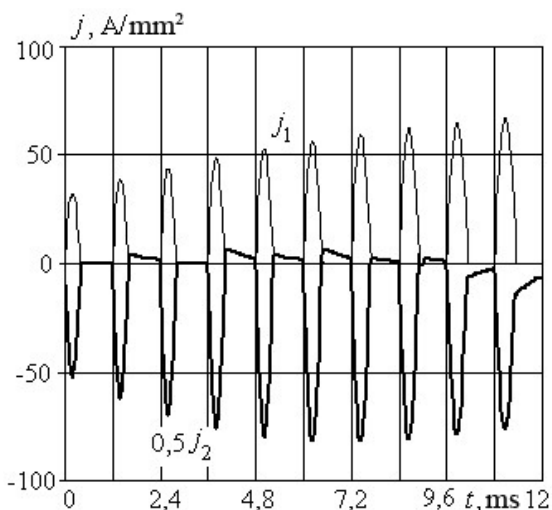
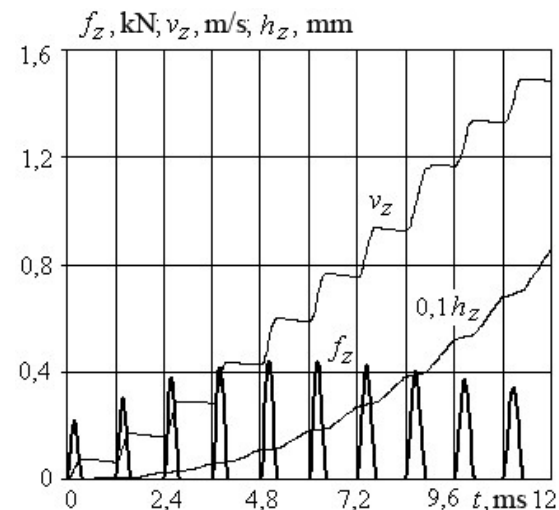


Fig. 3. Electromechanical characteristics of the IDC when excited by a packet of pulses from the CES sections of the same capacitance $C_0 = 100 \mu\text{F}$, charged to different voltages U_0



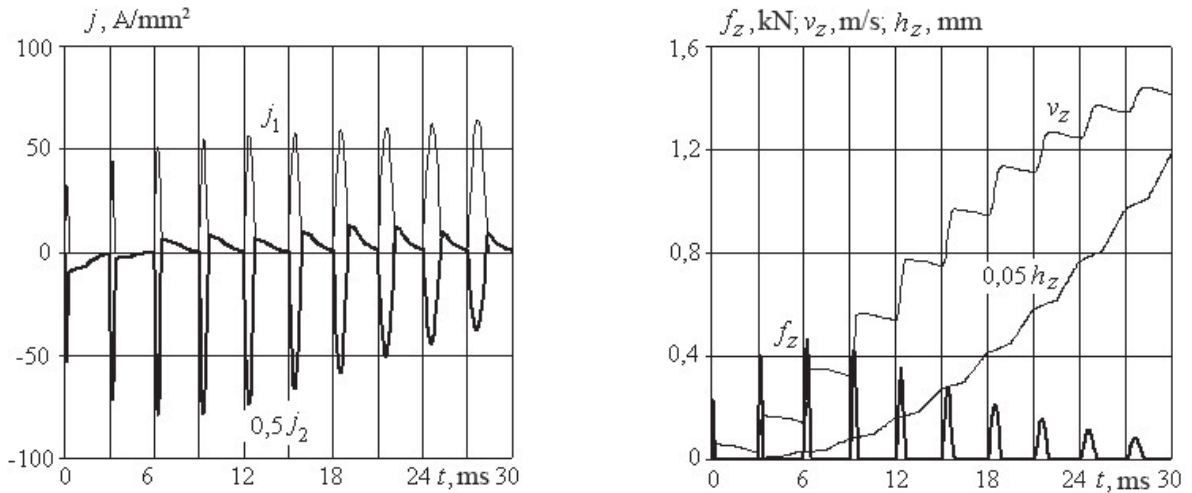


Fig. 4. Electromechanical characteristics of the IDC when excited by a packet of pulses with a period of 3 ms, from the CES sections charged to a voltage $U_0 = 210$ V, which capacity C_0 increases linearly

$h_z = 23.7$ mm. This packet of pulses provides pushing the armature to a height $h_{zm} = 126.2$ mm.

Thus, the excitation of the BLG catapult by a packet of sequential pulses provides the reduced auto seismic oscillations of the foundation by reducing the amplitudes of the EDF pulses and increasing the time of their effect. It is most appropriate to excite the IDC by the pulse packet from the CES sections of the same capacitance, but charged to a sequentially increased voltage, or from sections that have a sequentially increased capacitance, but charged to a single voltage.

Investigation of the efficiency of the multi-impulse method of excitation of the BLG induction-dynamic catapult

Let's consider the effect of excitation of the BLG induction-dynamic catapult by a pulse packet on the auto seismic uncertainty component (ASU) of the measurement of g in comparison with the excitation of the catapult by a single pulse. The value of the auto seismic uncertainty component of the measurement of g is estimated by modeling the mechanical system of the BLG [7, 15, 16]. When modeling, we use the following

parameters of the mechanical system of the BLG [15–17]: the foundation mass $m_0 = 3000$ kg, the stiffness of the soil base $c_0 = 125.88$ MN/m, the coefficient of viscous friction of the base $b_0 = 73743.2$ N · s/m; the TB mass $m = 0.08$ kg; the TB initial velocity $v = 1.4$ m/s (which corresponds to the push of the TB to a height of about 0.10 m).

An elastic suspension of the BLG interferometer reference reflector is used as a vibration protection system [17]. At this, the mass of the reference reflector is taken to be equal $m_v = 0.1$ kg, and the period of the proper oscillations of the vibration protection system is 10 s. We assume that the vibration protection system works in a critical mode. As an indicator of efficiency, we take the ASU of the GA measurement, which is determined by the expression [17]

$$\Delta g = -\sum_{k=0}^{K-1} x_v(kh + t_0 - \frac{T}{2}) \cdot w(k), \quad (11)$$

where $x_v(t)$ is the process of moving the reference reflector; h is the sampling interval of count processing of the path travelled by the TB; t_0 is the point of time when the TB reaches the top; $w(k)$ are the weighting

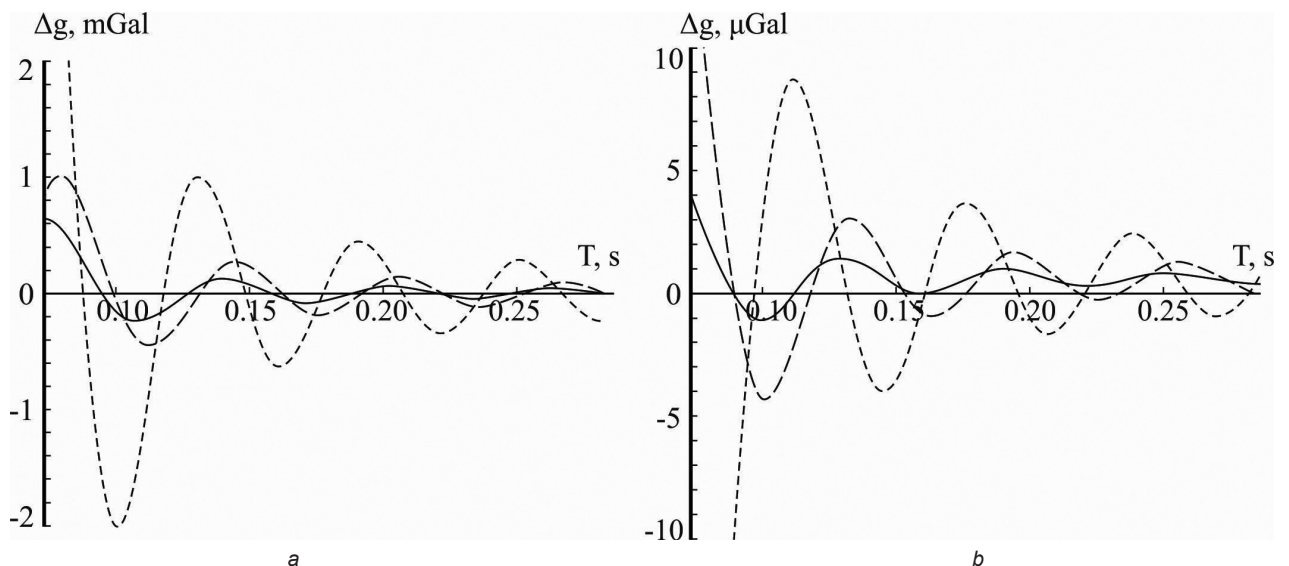


Fig. 5. Auto seismic uncertainty component of g measurement for the BLG without (a) and with (b) vibration protection

factors of path-time count processing in the BLG; T is the duration of the processing interval.

The sampling interval h in equation (11) we choose equal to 0.5 ms. At this, the processing factors $w(k)$ corresponding to the method of least squares are used.

The modeling results presented in the form of graphs in Fig. 5 (a), (b) show the dependences of the auto seismic uncertainty component of g measurement on the duration of the processing interval T . In this Fig., the curves correspond to different excitation signals of the BLG electrodynamic catapult: 1) a curve with a short dotted line – a single excitation pulse lasting 1 ms; 2) a curve with a long dotted line – a packet of ten pulses lasting 1 ms with a period between pulses 2 ms; 3) solid curve – a packet of ten pulses lasting 1 ms with a period between pulses 5 ms. The intensities of the excitation pulses in all three cases are chosen so as to provide the same initial velocity of the TB $v = 1.4$ m/s.

From the analysis of the obtained dependences of the ASU value of g measurement it is concluded that the transition from the method of excitation of the BLG induction-dynamic catapult with one short pulse to its excitation by the packet of pulses of the same duration allows to significantly reduce the uncertainty of g measurement by the gravimeter with the symmetric measurement method on account of reducing the auto seismic component of uncertainty in 3–5 times.

Conclusions

The mathematical model of the IDC describing interconnected electric, magnetic and mechanical processes is developed. It is found that when the IDC is excited by a packet of ten pulses, the duration of which is equal to 12 ms, from the CES sections with the same parameters, a consistent reduction in the amplitudes of the EDF pulses is observed. When the IDC is excited by a packet of pulses from the CES sections of the same capacitance, but charged to a voltage U_0 , which linearly increases, the amplitude of the EDF is the smallest in the first pulse, then it reaches a maximum value in the fifth pulse. When the IDC is excited by a packet of pulses from the CES sections charged to a voltage $U_0 = 210$ V, the capacitance C_0 of which increases linearly, the amplitude of the EDF reaches the highest value in the third pulse. Reducing the pulse period does not change the nature of the amplitudes of currents and the EDF in the catapult, but provides the pushing of the armature with the TB to a greater height.

The transition from the excitation method of the BLG induction-dynamic catapult with one short pulse to its excitation by a series of ten pulses of the same duration allows to significantly reduce the uncertainty of the GA measurement by the gravimeter with the symmetric measurement method by reducing the auto seismic component of the uncertainty of the GA measurement by 3–5 times.

Зменшення автосейсмічних коливань балістичного лазерного гравіметра за рахунок збудження індукційно-динамічної катапульти пакетом імпульсів

В.Ф. Болюх¹, О.І. Вінніченко², П.І. Неєжмаков², А.В. Омельченко³

¹ Національний технічний університет "Харківський політехнічний інститут", вул. Кирпичова, 2, 61002, Харків, Україна
bolyukh@gmail.com

² Національний науковий центр "Інститут метрології", вул. Мירוносицька, 42, 61002, Харків, Україна
vinnsc2@gmail.com

³ Харківський національний університет радіоелектроніки, пр. Науки, 14, 61166, Харків, Україна
otela5656@gmail.com

Анотація

Для зменшення автосейсмічних коливань у балістичних лазерних гравіметрах з симетричним методом вимірювання прискорення вільного падіння використовується індукційно-динамічна катапульта (ІДК), яка збуджується пакетом імпульсів від ємнісного накопичувача енергії. При такому збудженні досягається зменшення амплітуди автосейсмічних коливань за рахунок зменшення амплітуди та збільшення тривалості дії електродинамічної сили, яка виникає в індукційно-динамічній катапульти при підкиданні пробного тіла (ПТ).

Розроблено математичну модель індукційно-динамічної катапульти балістичного лазерного гравіметра з симетричним методом вимірювання прискорення вільного падіння та проведено моделювання її електромеханічних характеристик. Розглянуто різні способи формування пакету імпульсів збудження індуктора ІДК і для них досліджено характеристики імпульсів електродинамічних зусиль, що здійснюють розгін якоря катапульти з ПТ. Досліджено вплив збудження індукційно-динамічної катапульти пакетом імпульсів на автосейсмічну складову вимірювання прискорення вільного падіння. Показано, що за рахунок збудження індукційно-динамічної катапульти пакетом із

десяти імпульсів можна зменшити автосейсмічну складову невизначеності вимірювання прискорення вільного падіння балістичними гравіметрами в декілька (3–5) разів у порівнянні зі збудженням катапульти одиничним імпульсом.

Ключові слова: балістичний лазерний гравіметр; індукційно-динамічна катапульта; автосейсмічна складово невизначеності вимірювання.

Уменьшение автосейсмических колебаний баллистического лазерного гравиметра за счет возбуждения индукционно-динамической катапульти пакетом импульсов

В.Ф. Болух¹, А.И. Винниченко², П.И. Неежмаков², А.В. Омельченко³

¹ *Национальный технический университет “Харьковский политехнический институт”, ул. Кирпичева, 2, 61002, Харьков, Украина*

vfolyukh@gmail.com

² *Национальный научный центр “Институт метрологии”, ул. Мироносицкая, 42, 61002, Харьков, Украина*

vinnsc2@gmail.com

³ *Харьковский национальный университет радиозлектроники, пр. Науки, 14, 61166, Харьков, Украина*

omela5656@gmail.com

Аннотация

Для уменьшения автосейсмических колебаний в баллистическом лазерном гравиметре с симметричным методом измерения ускорения свободного падения (УСП) используется индукционно-динамическая катапульта (ИДК), которая возбуждается пакетом импульсов от емкостного накопителя энергии. При таком возбуждении достигается уменьшение амплитуды автосейсмических колебаний за счет уменьшения амплитуды и увеличения длительности действия электродинамической силы, которая возникает в ИДК при подбрасывании пробного тела.

Разработана математическая модель индукционно-динамической катапульти гравиметра с симметричным методом измерения УСП и выполнено моделирование ее электромеханических характеристик. Исследовано влияние возбуждения ИДК пакетом импульсов на автосейсмическую составляющую неопределенности измерения ускорения свободного падения. Показано, что за счет возбуждения ИДК пакетом из десяти импульсов можно уменьшить автосейсмическую составляющую неопределенности измерения УСП баллистическими гравиметрами в 3–5 раз в сравнении с возбуждением катапульти единичным импульсом.

Ключевые слова: баллистический лазерный гравиметр; индукционно-динамическая катапульта; автосейсмическая составляющая неопределенности измерения.

References

1. Vitushkin L.F., Orlov O.A., Dzhermak A., D’agostino D. Lazernyye interferometry peremeshcheniy s subnanometrovym razresheniyem v absolyutnykh ballisticheskikh gravimetrakh [Laser displacement interferometers with subnanometer resolution in absolute ballistic gravimeters]. *Measurement Techniques*, 2012, no. 3, pp. 3–8 (in Russian).
2. Niebauer T.M., Sasagawa G.S., Faller J.E. et al. A new generation of absolute gravimeters. *Metrologia*, 1995, no. 32, pp. 159–180.
3. Arnautov G.P. Rezultaty mezhdunarodnykh metrologicheskikh sravneniy absolyutnykh lazernykh ballisticheskikh gravimetrov [Results of international metrological comparisons of absolute laser ballistic gravimeters]. *Avtometriya*, 2005, vol. 41(1), pp. 126–136 (in Russian).
4. Bunin I.A., Kalish E.N., Nosov D.A., Smirnov M.G., Stus Yu.F. Polevoy absolyutnyy lazernyy ballisticheskyy gravimetr [Field absolute laser ballistic gravimeter]. *Avtometriya*, 2010, vol. 46(5), pp. 94–102 (in Russian).
5. Rothleitner Ch., Svitlov S., Merimeche H., Hu H., Wang L.J. Development of new free-fall absolute gravimeters. *Metrologia*, 2009, vol. 46(3), pp. 283–297. doi: 10.1088/0026-1394/46/3/017
6. Zanimonskiy Y.M., Nagornyy V.D. Ballisticheskyy gravimetr: podkhod v ramkakh teorii lineynykh sistem [Ballistic gravimeter: an approach within the linear systems theory]. *Measurement Techniques*, 1992, no. 3, pp. 34–36 (in Russian).
7. Bolyukh V.F., Omelchenko A.V., Vinnichenko A.I. Effect of self-seismic oscillations of the foundation on the readout of a ballistic gravimeter with an

- induction-dynamic catapult. *Measurement Techniques*, 2015, vol. 58(2), pp. 137–142.
8. Svitlov S.M. Metody analizu ta zmenshennia dynamichnykh pokhybok balistychnykh hравimetriv [Methods of analysis and reduction of dynamic errors of ballistic gravimeters]: author's abstract. Kharkiv, 2000. 17 p. (in Ukrainian).
 9. Bolyukh V.F., Vinnichenko A.I. Concept of an induction-dynamic catapult for a ballistic laser gravimeter. *Measurement Techniques*, 2014, vol. 56(10), pp. 1098–1104. doi: 10.1007/s11018-014-0337-z
 10. Bolyukh V.F., Katkov I.I. Influence of the Form of Pulse of Excitation on the Speed and Power Parameters of the Linear Pulse Electromechanical Converter of the Induction Type: Proceedings of ASME International Mechanical Engineering Congress and Exposition (IMECE), November 11–14, 2019. Vol. 2B: Advanced Manufacturing. No: IMECE2019-10388, V02BT02A047. Salt Lake City, Utah, USA, 2019. 8 p. <https://doi.org/10.1115/IMECE2019-10388>
 11. Bolyukh V.F., Kashanskyi Yu.V., Shchukin I.S. Sravnitelnyy analiz silovykh i skorostnykh pokazately lineynykh impulsnykh elektromekhanicheskikh preobrazovateley elektrodinamicheskogo i indukcionnogo tipov [Comparative analysis of power and speed indicators of linear pulse electromechanical converters of electrodynamic and induction types]. *Tekhnichna Elektrodynamika*, 2019, no. 6. pp. 35–42 (in Russian).
 12. Elsgolts L.E. Differentsialnyye uravneniya: uchebnik [Differential equations: a textbook]. Moscow, LKI, 2014. 312 p. (in Russian).
 13. Aleksandrova M.G., Belyanin A.N., Bryukner V. et al. Raschet elektricheskikh tsepey i elektromagnitnykh poley na EVM [Calculation of electrical circuits and electromagnetic fields on an electronic computing machine]. Moscow, *Radio i svyaz*, 1983. 344 p. (in Russian).
 14. Kalantarov P.L., Tseytlin L.A. Raschet induktivnostey: spravochnaya kniga [Calculation of inductances: a reference book]. Leningrad, Energoatomizdat, 1986. 488 p. (in Russian).
 15. Omelchenko A.V., Bolyukh V.F., Vinnichenko O.I. Avtoseismichna skladova pokhybky symetrychnoho balistychnoho hравimetra, zumovlena kolyvanniamy fundamentu [Autoseismic component of the error of symmetric ballistic gravimeter caused by foundation oscillations]. *Metrology and Instruments*, 2014, no. 3 (47), pp. 51–56 (in Ukrainian).
 16. Vinnichenko O., Neyezhnikov P., Omelchenko A., Fedorov O., Bolyukh V. Analiz vplyviv seismichnykh zavad na rezultaty vymiriuvannya pryskorennia vilnoho padinnia balistychnymy lazernymy hравimetramy [Analysis of the effects of seismic interference on the measurement results of gravitational acceleration by ballistic laser gravimeters]. *Ukrainian Merological Journal*, 2020, no. 1, pp. 51–61 (in Ukrainian). doi: 10.24027/2306-7039.1.2020.204228
 17. Bolyukh V.F., Omelchenko A.V., Vinnichenko A.I. A ballistic laser gravimeter for a symmetrical measurement method with the inductive-dynamic catapult and auto-seismic vibration preventing. *Static and Mobile Measurements (TG-SMM-2016): Proceedings of 4th IAG Symposium on Terrestrial Gravimetry*, April 12–15, 2016. Code 121590. State Research Center of the Russian Federation. Saint Petersburg, Russian Federation, 2016, pp. 113–118.